

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

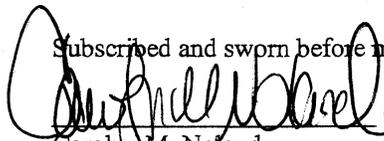
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130112 ✓			
Name	Bruce Smith Jr	ID#	3522	Date	4-3-09 ✓	
A	Agency	Wrangell Police Department	Phone #	(907) 874-3304		
Instrument Location		Wrangell Police Department, 431 Zimovia Highway ✓				
Alco S/N		X301583 ✓	Target Value	.080 ✓	High Pressure	350
B	Alco Test Values	.085 ✓	1 <sup>st</sup> Alco	.085 ✓	2 <sup>nd</sup> Alco	
Signature						
(OVER)						

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22 day of May 2009.  
 (Notary Seal Stamp)  
Carolyn M. Nofand  
Notary Public, State of Alaska  
Commission Expires with Office



APR 10 2009

BT9 06/03

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130112

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130112

APRIL 03, 2009

OPERATOR'S NAME:  
SMITH JR, BRUCE W  
OPERATOR'S NUMBER: 3522  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/NI :  
CAL

O.L. #: 0123456  
DEPT/AGENCY: WRG1  
CASE/REPORT: 09040000  
TEST TYPE: U  
ALCO TARGET VALUE: .000 ✓  
ALCO S/N: X301583 ✓

### — BREATH ANALYSIS —

.000 ADJUSTED FOR 30.29 in  
ALCO TARGET .000 16:46  
BLANK TEST .000 16:47  
INTERNAL STANDARD VERIFIED 16:47  
ALCO TV 30.29 in .005 ✓ 16:47  
BLANK TEST .000 16:48  
SUBJECT SAMPLE .000 16:49  
BLANK TEST .000 16:49  
ALCO TV 30.29 in .005 ✓ 16:50  
BLANK TEST .000 16:50

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130112

APRIL 03, 2009 ✓  
TIME 16:44

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 40c  
BREATH TUBE: 43c  
BAROMETER: 30.29 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { } ~ |