

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUL 15 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130112 ✓			
Name	Bruce Smith Jr	ID#	3522 ✓			
		Date	7-8-10 ✓			
A	Agency	Wrangell Police Department	Phone # (907) 874-3304			
	Instrument Location	Wrangell Police Department, 431 Zimovia Highway				
B	Alco S/N	77199 ✓	Target Value	0.083 ✓	High Pressure	600
	Alco Test Values	0.089 ✓	0.088 ✓			
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco			
	Signature					

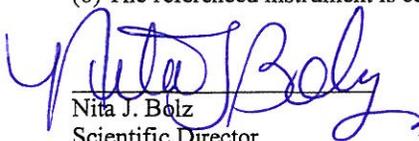
(OVER)

(Do Not write in the area below)

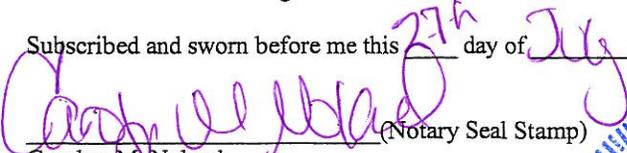
  
7/15/10


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 27<sup>th</sup> day of July, 2010.

  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N 130112

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

**NONDRINKING SUBJECT TEST**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130112

JULY 08, 2010

OPERATOR'S NAME:  
 SMITH JR, BRUCE W  
 OPERATOR'S NUMBER: 3522  
 SUBJECT'S LAST NAME:  
 UOC  
 SUBJECT'S FIRST NAME/NI :  
 UOC  
 O.L. #: 0123456  
 DEPT/AGENCY: WR61  
 CASE/REPORT:  
 TEST TYPE: U  
 ALCO TARGET VALUE: .003  
 ALCO S/N: 77199

--- BREATH ANALYSIS ---

.003 ADJUSTED FOR 30.38 in		
ALCO TARGET	.004	14:21
BLANK TEST	.000	14:21
INTERNAL STANDARD	VERIFIED	14:22
ALCO TV 30.38 in	.009	14:22
BLANK TEST	.000	14:23
SUBJECT SAMPLE	.000	14:23
BLANK TEST	.000	14:24
ALCO TV 30.38 in	.008	14:24
BLANK TEST	.000	14:25

**DIAGNOSTIC CHECK**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130112

JULY 08, 2010  
 TIME 14:19

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	40c
BREATH TUBE:	41c
BAROMETER:	30.38 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

```
!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abode+ghi jklmno
pqrstuvwxyz{|}~!@
```