

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


Supervisor/Operator Performing the Verification Procedure: <span style="float: right;">DataMaster cdm S/N <u>130112</u> ✓</span>					
Name <u>Bruce Smith Jr</u>	ID# <u>3522</u> ✓ Date <u>11-12-10</u> ✓				
A Agency <u>Wrangell Police Department</u> Phone # <u>(907) 874-3304</u>					
Instrument Location <u>Wrangell Police Department, 431 Zimovia Highway</u>					
B Alco S/N <u>X301542</u> ✓ Target Value <u>.077</u> ✓ High Pressure <u>1150</u>					
Alco Test Values	<table style="width:100%; border: none;"> <tr> <td style="text-align: center; border-bottom: 1px solid black;"><u>.083</u> ✓</td> <td style="text-align: center; border-bottom: 1px solid black;"><u>.083</u> ✓</td> </tr> <tr> <td style="text-align: center; font-size: small;">1<sup>st</sup> Alco</td> <td style="text-align: center; font-size: small;">2<sup>nd</sup> Alco</td> </tr> </table>	<u>.083</u> ✓	<u>.083</u> ✓	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
<u>.083</u> ✓	<u>.083</u> ✓				
1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco				
Signature <u></u>					
(OVER)					

*BMB*  
*12/16/10*

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

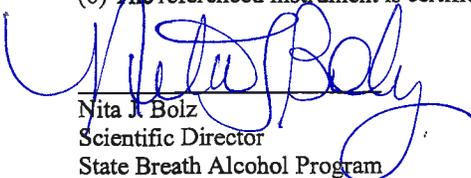  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>RD</sup> day of DEC, 2010.

 (Notary Seal Stamp)  
 Carolyn M. Noland **DANIEL NICHOLAS**  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130112

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130112

NOVEMBER 12, 2010

OPERATOR'S NAME:

SAITH JR, BRUCE W

OPERATOR'S NUMBER: 3522

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: 0123456

DEPT/AGENCY: WRG1

CASE/REPORT: 10110000

TEST TYPE: U

ALCO TARGET VALUE: .077

ALCO S/N: X301542

— BREATH ANALYSIS —

.077 ADJUSTED FOR 29.91 in

ALCO TARGET	.076	19:57
BLANK TEST	.000	19:58
INTERNAL STANDARD	VERIFIED	19:58
ALCO TV 29.90 in	.083	19:59
BLANK TEST	.000	20:00
SUBJECT SAMPLE	.000	20:00
BLANK TEST	.000	20:01
ALCO TV 29.91 in	.083	20:01
BLANK TEST	.000	20:02

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130112

NOVEMBER 12, 2010

TIME 19:55

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 29.91 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~