

JUN 03 2011

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | | | |
|--|---------------------|--|-------------------------------------|
| Supervisor/Operator Performing the Verification Procedure: | | DataMaster cdm S/N | 130113 |
| A | Name | Kenneth G. Cox | ID# 3527 Date <u>May 29, 2011</u> |
| | Agency | Skagway Police Department | Phone # (907) 983-2232 |
| | Instrument Location | Skagway Police Department 1st and State Street Skagway, AK 99840 | |
| B | Alco S/N | X173019 | Target Value .082 High Pressure 800 |
| | Alco Test Values | <u>.80</u> 1st Alco | <u>.80</u> 2 nd Alco |
| | Signature |  | |

28 NFB 6/16/11


(OVER)

NFB 6/13/11

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

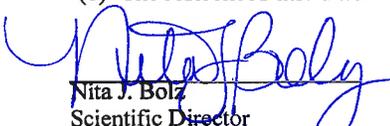
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 16 day of JUNE, 2011.


 Daniel L. Nicholas KYLE KLOPPER
 Notary Public, State of Alaska
 Commission Expires with Office

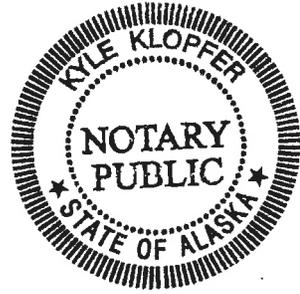

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130113

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113

MAY 28, 2011

OPERATOR'S NAME:
COX/KENNETH/G
OPERATOR'S NUMBER: 3527
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :

L
O.L. #: L
DEPT/AGENCY: SKGI
CASE/REPORT: 2011----
TEST TYPE: V
ALCO TARGET VALUE: .002
ALCO S/N: X173019

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 30.20 in
ALCO TARGET .002 16:57
BLANK TEST .000 16:58
INTERNAL STANDARD VERIFIED 16:58
ALCO TO 30.20 in .000 16:59
BLANK TEST .000 17:00
SUBJECT SAMPLE .000 17:01
BLANK TEST .000 17:01
ALCO TO 30.20 in .000 17:02
BLANK TEST .000 17:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY,
DATAMASTER cdm 130113

MAY 28, 2011
TIME 16:50

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: SKI
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 40c
BREATH TUBE: 42c
BAROMETER: 30.20 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNPOQRSTUVWXYZ[\]^_`abodefghi.jklmno
pqrstuvwxyz{|}~

