

FEB 06 2012

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

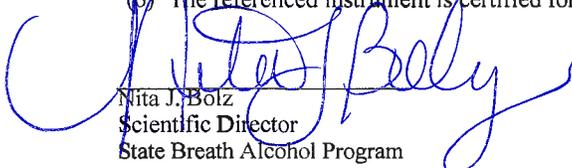
DataMaster cdm S/N _____ 130113	
Supervisor/Operator Performing the Verification Procedure:	
Name _____ Kenneth G. Cox	ID# 3527 Date 01/27/2012
A Agency _____ Skagway Police Department Phone # (907) 983-2232	
Instrument Location _____ Skagway Police Department 1st and State Street Skagway, AK 99840	
B Alco S/N _____ 4N Target Value _____ .080 High Pressure _____ 1000 psi	
Alco Test Values	_____ .082 _____ .081
	1st Alco 2nd Alco
Signature _____	COB 2/6/12

(OVER)



(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, ~~2010~~ ²⁰¹²  4/5/12


 Daniel E. Nicholas 
 Notary Public, State of Alaska
 Commission Expires with Office 4/5/12



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130113

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113

JANUARY 27, 2012

OPERATOR'S NAME:

COB
9/16/12
COB/KENNETH/S

OPERATOR'S NUMBER: 3527

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: SK61

CASE/REPORT: 2012-0131

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: 4N

— BREATH ANALYSIS —

.000 ADJUSTED FOR 30.09 in
ALCO TARGET .000 13:32
BLANK TEST .000 13:34
INTERNAL STANDARD VERIFIED 13:34
ALCO TV 30.09 in .002 13:34
BLANK TEST .000 13:35
SUBJECT SAMPLE .000 13:35
BLANK TEST .000 13:36
ALCO TV 30.09 in .001 13:37
BLANK TEST .000 13:37

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113

JANUARY 27, 2012
TIME 13:39

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 30.09 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=?@ABCDEF6
HIJKLNPQRSTUWXYZ[\]^_`abcdefgijklmnop
qprstuvwxyz{|}~■

