

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 08 2010

DataMaster cdm S/N: 130113

Supervisor/Operator Performing the Verification Procedure:

Name: Kenneth G. Cox ID #: 3527 Date: February 28, 2010

A Agency: Skagway Police Department Phone #: 907 983-2232

Instrument Location Skagway Police Department, 1st & State Street Skagway, Alaska 99840

Alco S/N X173010 Target Value .082 High Pressure 300

Alco Test Value Average .081 0.080 6-8-10 COB
1st Alco 2nd Alco

Signature [Handwritten Signature] COB
3/11/10

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Handwritten Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 23rd day of March, 2010.

[Handwritten Signature]
(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

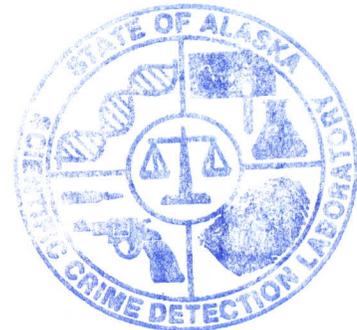

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130113

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113 ✓

FEBRUARY 28, 2010 ✓

OPERATOR'S NAME: *CSB 3/11/10*
COX/KENNETH/G
OPERATOR'S NUMBER: 3527
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
L

O.L. #: L
DEPT/AGENCY: SK61 ✓
CASE/REPORT: 2010-0331 ✓
TEST TYPE: U ✓
ALCO S/N: X173010 ✓

— BREATH ANALYSIS —

.082 ADJUSTED FOR 29.59 in		
ALCO TARGET	.081	15:40
BLANK TEST	.000	15:41
INTERNAL STANDARD	VERIFIED	15:41
ALCO TV 29.59 in	.080 ✓	15:41
BLANK TEST	.000	15:42
SUBJECT SAMPLE	.000 ✓	15:42
BLANK TEST	.000	15:43
ALCO TV 29.59 in	.081 ✓	15:44
BLANK TEST	.000	15:44

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113 ✓

FEBRUARY 28, 2010 ✓
TIME 15:35

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.59 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~