

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

FEB 18 2009

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130114</u> ✓
A	Name <u>Kevin Stevenson</u>	ID# <u>2414</u> Date <u>02-15-09</u> ✓
	Agency <u>WAA Police Dept</u>	Phone # <u>907-786-1120</u>
	Instrument Location <u>WAA Police Dept DUI PROCESSING</u> ✓	
B	Alco S/N <u>X301591</u> ✓	Target Value <u>0.080</u> ✓ High Pressure <u>500</u>
	Alco Test Value Average <u>.078</u> ✓	<u>.078</u> ✓
	1 st Alco	2 nd Alco
	Signature <u>[Handwritten Signature]</u> ✓	<u>CAB</u> <u>2/23/09</u>


Under the Alaska Rules of Evidence, I certify that, (OVER)

(Do Not write in the area below)
(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kevin Stevenson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

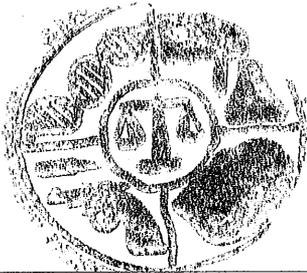

[Handwritten Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

2/23/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114

FEBRUARY 15, 2009

OPERATOR'S NAME:

STEVENSON KEVIN L

OPERATOR'S NUMBER: 2414

SUBJECT'S LAST NAME:

VERIFICATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION

O.L. #: 21234

DEPT/AGENCY: ANC7

CASE/REPORT: 0908

TEST TYPE: U

ALCO TARGET VALUE: .000 ✓

ALCO S/N: X301591 ✓

— BREATH ANALYSIS —

.000 ADJUSTED FOR 29.67 in
ALCO TARGET .079 17:14
BLANK TEST .000 17:15
INTERNAL STANDARD VERIFIED 17:15
ALCO TV 29.67 in .078 ✓ 17:15
BLANK TEST .000 17:16
SUBJECT SAMPLE .000 17:17
BLANK TEST .000 17:18
ALCO TV 29.67 in .078 ✓ 17:18
BLANK TEST .000 17:19

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114

FEBRUARY 15, 2009 ✓

TIME 17:11

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.67 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNPOQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~