

MAR 05 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130114</u>
Name		<u>J Swartz</u>	ID# <u>4314</u> Date <u>12/08/07</u>
A	Agency	<u>SCDL</u>	Phone # <u>269-5592</u>
Instrument Location		<u>SCDL</u>	
Alco S/N		<u>SCOTT07</u>	Target Value <u>.080</u> High Pressure <u>600 psi</u>
Alco Test Values		<u>.078</u>	<u>.077</u>
		1 st Alco	2 nd Alco
Signature		<u>[Signature]</u>	<u>[Signature]</u> <u>3/6/08</u>

(OVER)

Under the Alaska Rules of Evidence, I certify that;

(Do Not write in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jeanne M Swartz, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed



[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/6/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm-breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114


(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

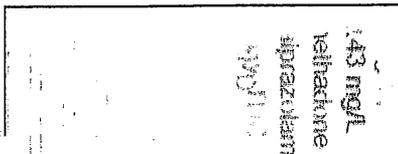

DIAGNOSTIC CHECK

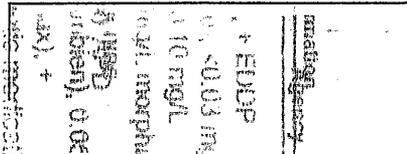

Breath Test Record

Serial Number	130114	Model	DataMaster
Location	ANC1	Anchorage Police Dept.	

Subject Information

Last Name	Verification Of Cal	O.L. #	L
First Name	L		

Operator Information

Operator Name	Swartz/J	Case	
Operator #	4314	Department	AAA1

Test Results

Alco Target	0.08	Alco Serial	SCOTT07		
Nominal	0.079	Barometer	29.68	Test Type	<input checked="" type="checkbox"/>
Dry Gas 1	0.078	Time:	07:42:38	Test Date	12/08/2007
Subject Alcohol	0.000	Time:	07:44:24	Test Time	07:41:10
Dry Gas 2	0.077	Time:	07:45:30	Report	<input checked="" type="checkbox"/>

Diagnostic Test Record

Serial Number	130114	Model	DataMaster
Location	ANC1	Anchorage Police Dept.	

Diagnostic Test Results

Test Date	12/08/2007	Computer	Okay
Test Time	07:32:08	Program	Okay
Software Date	02/20/2001	Sample Chamber (C)	49
Breath Tube (C)	42	Barometer (in)	29.68
Flow Detector	Okay	High Speed Pump	Okay
Detector	Okay	Filter	Okay
Quartz	Okay	Calibration	Okay