

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 17 2010

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130114

Name Kevin Stevenson ID# 2411 Date 05-12-10

A Agency WAA Police Dept Phone # 786-1120

Instrument Location \_\_\_\_\_

B Alco S/N 75470 Target Value .080 High Pressure 500

Alco Test Value Average .081 .082  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature] CIB  
5/24/10



(OVER)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 17<sup>th</sup> day of June, 2010.  
[Signature] (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

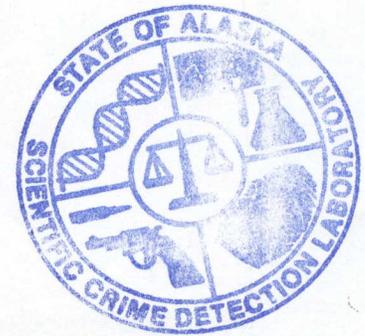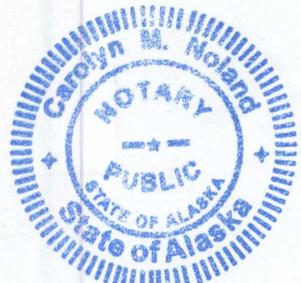

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130114

MAY 12, 2010

OPERATOR'S NAME: **CB 5/24/10**  
STEVENS ON KEVIN L  
OPERATOR'S NUMBER: 2414  
SUBJECT'S LAST NAME:  
VERIFICATION  
SUBJECT'S FIRST NAME (M) :  
VERIFICATION  
O.L. #: 12345  
DEPT/AGENCY: ANCP  
CASE # (S/C/T): 1029472  
TEST TYPE: U  
ALCO TARGET VALUE: .080  
ALCO S/N: 75470

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 29.83 in		
ALCO TARGET	.079	22:06
BLANK TEST	.000	22:07
INTERNAL STANDARD	SPITTED	22:07
ALCO TU 29.83 in	011	22:07
BLANK TEST	000	22:08
SUBJECT SAMPLE	000	22:08
BLANK TEST	000	22:09
ALCO TU 29.83 in	002	22:10
BLANK TEST	000	22:10

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130114

MAY 12, 2010  
TIME 22:03

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/09/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 49c  
BAROMETER: 29.83 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./:;<=>?@AB CDEFG  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~