VERIFICATION OF CALIBRATION REPORT

NOV 1 2 2010

of DataMaster cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114 ✓

Supervisor/Operator Performing the Verification Procedure:

A

Name Kevin Stevenson ID# 2414 ✓ Date 11-5-10 ✓

Agency UAA Police Dept Phone # 786-1120

Instrument Location UAA Police Dept Eugene Shot Hall Suite 114

B

Alco S/N G30491 ✓ Target Value .079 ✓ High Pressure 1100

Alco Test Values .077 ✓ (1st Alco) .077 ✓ (2nd Alco)

Signature [signature]

(OVER)

BMB 12/8/10

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
(3) I am the Scientific Director of the State Breath Alcohol Program.
(4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
(5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 23RD day of DEC, 2010.

[signature] (Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

DANIEL L. NICHOLAS Commission # 116780 NOTARY PUBLIC My Commission Expires With Office STATE OF ALASKA

STATE OF ALASKA DEPARTMENT OF PUBLIC SAFETY SCIENTIFIC CRIME DETECTION LABORATORY

BT9 06/03

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST
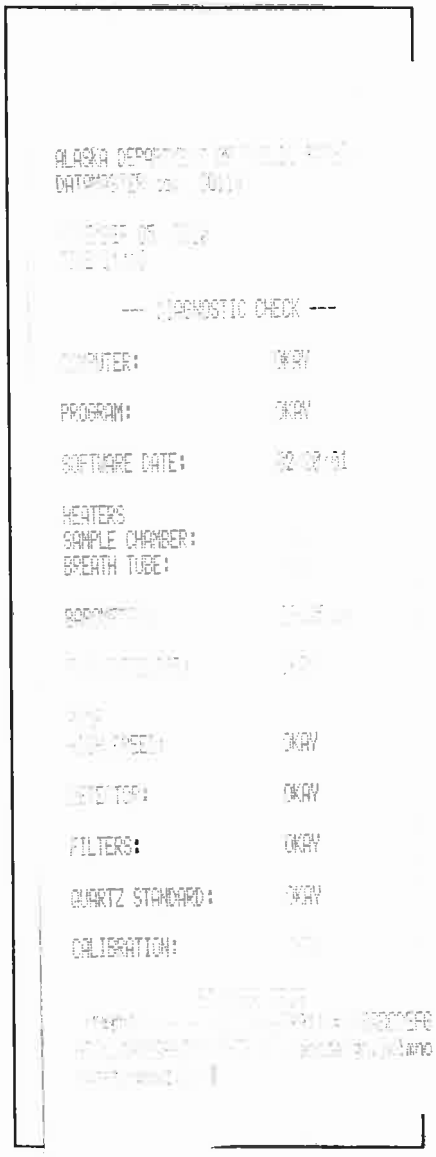
DIAGNOSTIC CHECK