

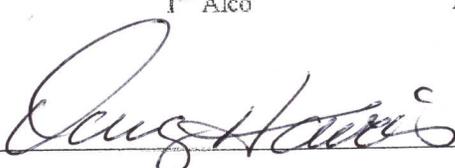
VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

MAR 04 2010

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

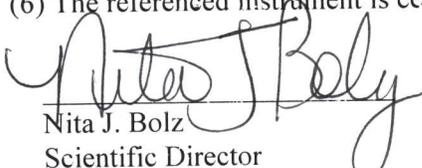
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130115 ✓		
Name	DOUG E. HARRIS	ID#	5530	Date	3-2-2010 ✓
Agency	BRISTOL BAY POLICE		Phone #	907-246-4222	
Instrument Location	BBPD BLDG 150 KSAFB KING SALMON AK ✓				
Alco S/N	X301605 ✓	Target Value	.075 ✓	High Pressure	
Alco Test Values	.073 ✓ 1 st Alco		.072 ✓ 2 nd Alco		
Signature					
(OVER)					

BMB
3/18/2010

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of March, 2010.

(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130115 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130115

MARCH 02, 2010

OPERATOR'S NAME:

HARRIS DOUG E

OPERATOR'S NUMBER: 5538

SUBJECT'S LAST NAME:

SUBJECT'S FIRST NAME/MI :

ALASKA DEPARTMENT OF PUBLIC SAFETY

DEPARTMENTAL UNIT

DATE RECEIVED: 03/02/10

TEST MODE: 11

ALCOHOL CALIBRATION: 075 ✓

ALCOHOL CALIBRATION

--- BREATH ANALYSIS ---

ALCOHOL TESTED FOR 20.37 in

ALCOHOL TESTED FOR 0.072 16:00

ALCOHOL TESTED FOR 0.000 16:01

ALCOHOL TESTED FOR VERIFIED 16:01

ALCOHOL TESTED FOR 0.000 16:02

ALCOHOL TESTED FOR 0.000 16:03

ALCOHOL TESTED FOR 0.000 16:03

ALCOHOL TESTED FOR 0.000 16:04

ALCOHOL TESTED FOR 0.000 16:04

ALCOHOL TESTED FOR 0.000 16:05

BMB
3/18/2010

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130115

MARCH 02, 2010

TIME 15:45

--- DIAGNOSTIC CHECK ---

ALCOHOL TESTED FOR 0.000

ALCOHOL TESTED FOR 0.000

ALCOHOL TESTED FOR 0.000/0.01

ALCOHOL TESTED FOR 0.000

ALCOHOL TESTED FOR 0.000

ALCOHOL TESTED FOR 0.000

ALCOHOL TESTED FOR 0.000 in

ALCOHOL TESTED FOR 0.000

PRINTER TEST

ALCOHOL TESTED FOR 0.000 (=)0000000000

ALCOHOL TESTED FOR 0.000 (=)0000000000