

# VERIFICATION OF CALIBRATION REPORT APR 15 2010

of DataMaster edm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster edm S/N <u>130115</u> ✓	
Name <u>DOUG E. HARRIS</u>	ID# <u>5530</u> Date <u>4-11-2010</u> ✓
Agency <u>BRISTOL BAY POLICE</u>	Phone # <u>246-4222</u>
Instrument Location <u>BBPD</u> ✓	
Alco S/N <u>X301605</u> ✓ Target Value <u>.075</u> ✓ High Pressure _____	
Alco Test Values 1 <sup>st</sup> Alco <u>.075</u> ✓      2 <sup>nd</sup> Alco <u>.075</u> ✓	
Signature <u><i>Doug Harris</i></u> ✓	<u>COB</u> <u>4/26/10</u>
(OVER)	

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of April, 2010.

*Carolyn M. Noland* (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

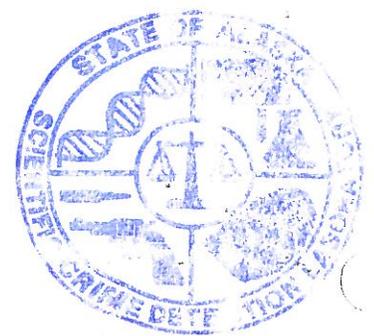

# VERIFICATION OF CALIBRATION REPORT

of DataMaster edm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster edm S/N 130115

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130115

APRIL 11, 2010

OPERATOR'S NAME:

HARRIS DOUG E

OPERATOR'S NUMBER: 5330

SUBJECT'S LAST NAME:

TEST

SUBJECT'S FIRST NAME/MI :

TEST

O.L. #: 0101010

DEPT/AGENCY: NKN1

CRSE/REPORT: 000000

TEST TYPE: U

ALCO TARGET VALUE: 075

ALCO S/N: X001625

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 29.98 in  
ALCO TARGET .075 16:02  
BLANK TEST .000 16:03  
INTERNAL STANDARD VERIFIED 16:03  
ALCO TO 29.98 in .075 16:04  
BLANK TEST .000 16:05  
SUBJECT SAMPLE .000 16:05  
BLANK TEST .000 16:06  
ALCO TO 29.98 in .075 16:06  
BLANK TEST .000 16:07

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130115

APRIL 11, 2010

TIME 16:08

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/28/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
PARAMETERS: 29.98 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTRATION: OKAY  
GLASS STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

0123-5678910(=>?@#CDEF6  
ABCDEFGHIJKLNO  
PQRSTUVWXYZ