

# VERIFICATION OF CALIBRATION REPORT

of DataMaster edm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster edm S/N 130116 ✓

Name Kenneth Parker ID# 5578 Date 02/15/08

Agency McGrath Public Safety Phone # 324-3095

Instrument Location AST

---

Alco S/N 77111 ✓ Target Value 0.078 ✓ High Pressure 1.900

Alco Test Values

	<u>0.074</u>	<u>0.074</u>
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco

Signature [Signature] 02/15/08

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kenneth Parker, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

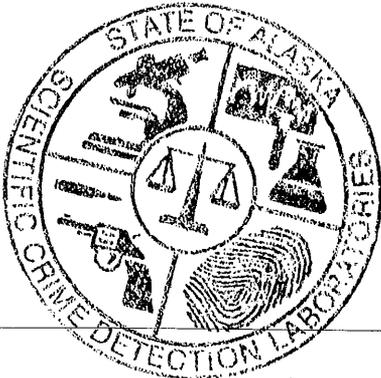

Signed and sealed.

[Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/1/08  
Date

FEB 25 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130116

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130116

FEBRUARY 15, 2008

OPERATOR'S NAME: PARKER/KENNETH/W  
OPERATOR'S NUMBER: 5578  
SUBJECT'S LAST NAME: PARKER

SUBJECT'S FIRST NAME/MI: KENNETH/W

O.L. #: 130116  
DEPT/AGENCY: MCGRI  
CASE/REPORT: T

TEST TYPE: T  
ALCO TARGET VALUE: 078  
ALCO S/N: 77111

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.62 in		
ALCO TARGET	.077	10:19
BLANK TEST	.000	10:20
INTERNAL STANDARD	VERIFIED	10:21
ALCO TU 29.62 in	.074	10:21
BLANK TEST	.000	10:22
SUBJECT SAMPLE	.000	10:22
BLANK TEST	.000	10:23
ALCO TU 29.62 in	.074	10:24
BLANK TEST	.000	10:24

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130116

FEBRUARY 15, 2008  
TIME 10:15

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	40c
BAROMETER:	29.62 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~■