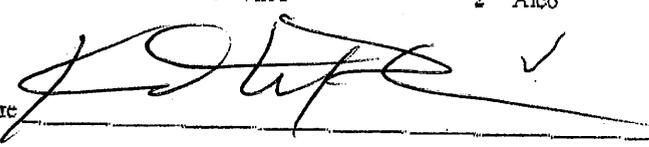


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130116</u> ✓
Name	<u>Kenneth Parker</u>	ID# <u>5578</u> Date <u>08-15-08</u> ✓
Agency	<u>McGrath Public Safety</u> ✓	Phone # <u>524-3075</u>
Instrument Location	<u>Capt Snow Building</u> ✓	
Alco S/N	<u>77111</u> ✓	Target Value <u>.078</u> ✓ High Pressure <u>850</u>
Alco Test Values	<u>.075</u> ✓ 1 st Alco	<u>.074</u> ✓ 2 nd Alco
Signature	 ✓	<u>CSB</u> <u>8/18/08</u>

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kenneth Parker, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

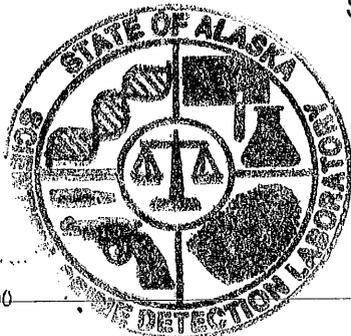



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

8/20/08
Date

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 13 0116 v

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130116

AUGUST 15, 2008

OPERATOR'S NAME:
PARKER/KENNETH/W
OPERATOR'S NUMBER: 5578
SUBJECT'S LAST NAME:
PARKER
SUBJECT'S FIRST NAME/MI :
KENNETH/W

O.L. #: 130116
DEPT/AGENCY: MCGI
CASE/REPORT: T
TEST TYPE: T
ALCO TARGET VALUE: 078 ✓
ALCO S/N: 77111 ✓

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.85 in		
ALCO TARGET	.077	11:11
BLANK TEST	.000	11:12
INTERNAL STANDARD	VERIFIED	11:12
ALCO TV 29.85 in	.075	11:13
BLANK TEST	.000	11:14
SUBJECT SAMPLE	.000	11:14
BLANK TEST	.000	11:15
ALCO TV 29.85 in	.074	11:16
BLANK TEST	.000	11:16

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130116

AUGUST 15, 2008 ✓
TIME 11:01

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.85 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; (=) ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¯