

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130116 ✓

Supervisor/Operator Performing the Verification Procedure:
 Name Michael Carpenter ID# 6714 ✓ Date 10-3-10 ✓
 A Agency Alaska State Troopers Phone # 524-3052
 Instrument Location McGrath State Trooper Post

B Alco S/N 77111 ✓ Target Value .078 ✓ High Pressure 700
 Alco Test Values .071 ✓ 1st Alco .072 ✓ 2nd Alco
 Signature [Handwritten Signatures]

(OVER)

BMB
12/8/10

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Handwritten Signature]
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 16th day of DEC, 2010.

[Handwritten Signature] (Notary Seal Stamp)
 Daniel L. Nicholas
 Notary Public, State of Alaska
 Commission Expires with Office

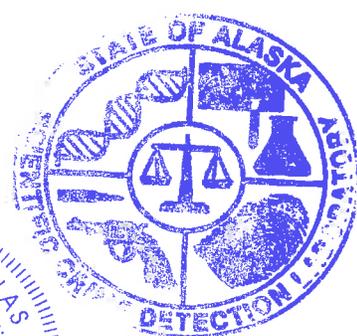

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130116

BMB
12/8/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST



ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130116

OCTOBER 03, 2010

OPERATOR'S NAME:
CARPENTER
OPERATOR'S NUMBER: 6714
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
L

BMB
12/8/10

O.L. #: L
DEPT/AGENCY: MC60
CASE/REPORT:
TEST TYPE: D
ALCO TARGET VALUE: .078
ALCO S/N: 77111

— BREATH ANALYSIS —

.078 ADJUSTED FOR 29.25 in
ALCO TARGET .076 10:30
BLANK TEST .000 10:31
INTERNAL STANDARD VERIFIED 10:31
ALCO TU 29.25 in .071 10:31
BLANK TEST .000 10:32
SUBJECT SAMPLE .000 10:33
BLANK TEST .000 10:34
ALCO TU 29.25 in .072 10:34
BLANK TEST .000 10:35

BMB
12/8/10



DIAGNOSTIC CHECK



ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130116

OCTOBER 03, 2010
TIME 10:24

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 40c
BAROMETER: 29.25 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢