

MAR 13 2008

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


DataMaster cdm S/N <u>130117</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>KYLE VALERIO</u>	ID# <u>2093</u> Date <u>3-12-2008</u> ✓
A Agency <u>KODIAK POLICE DEPARTMENT</u> Phone # <u>(907)486-8000</u>	
Instrument Location <u>217 LOWER MILL BAY ROAD, KODIAK, AK. 99615</u>	
B Alco S/N <u>58442</u> ✓ Target Value <u>.081</u> ✓ High Pressure <u>1200</u>	
Alco Test Values	<u>.077</u> <u>.076</u> 1 <sup>st</sup> Alco                                      2 <sup>nd</sup> Alco
Signature 	<u>CSB</u> <u>3/18/08</u>
(OVER)	

(Do Not write in the area below)  
Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kyle Valerio, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

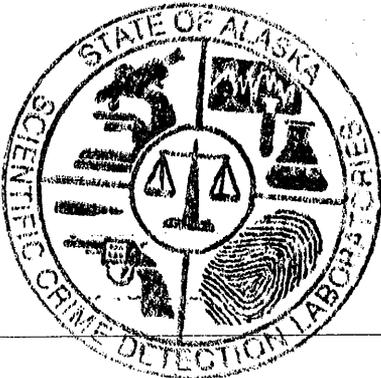

Signed and sealed,



Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/18/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130117

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130117

MARCH 12, 2008

OPERATOR'S NAME: *COS 3/18/08*  
VALERIO, KVLE D  
OPERATOR'S NUMBER: 2093  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
TEST

O.L. #: XXXXXXX  
DEPT/AGENCY: KOD1  
CASE/REPORT: 20000000  
TEST TYPE: U  
ALCO TARGET VALUE: .081  
ALCO S/N: 58442

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.12 in  
ALCO TARGET .081 05:46  
BLANK TEST .000 05:47  
INTERNAL STANDARD VERIFIED 05:48  
ALCO TV 30.12 in .077 05:48  
BLANK TEST .000 05:49  
SUBJECT SAMPLE .000 *COS 3/18/08* 05:49  
BLANK TEST .000 05:50  
ALCO TV 30.12 in .076 05:50  
BLANK TEST .000 05:51

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130117

MARCH 12, 2008  
TIME 05:52

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.12 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { } ~ #