


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 22 2009

|  |   |
|--|---|
| DataMaster cdm S/N <u>130117</u>   |   |
| Supervisor/Operator Performing the Verification Procedure:                                   |   |
| Name <u>KYLE VALERIO</u>   | ID# <u>2093</u> Date <u>10/13/2009</u>  |
| <b>A</b>   |   |
| Agency <u>KODIAK POLICE DEPARTMENT</u>   | Phone # <u>(907)486-8000</u>  |
| Instrument Location <u>217 LOWER MILL BAY ROAD, KODIAK, AK. 99615</u>                        |   |
| <b>B</b>   |   |
| Alco S/N <u>X172938</u>  | Target Value <u>.087</u> High Pressure <u>950</u>                                   |
| Alco Test Values   | <u>.083</u> <u>.084</u>   |
| 1 <sup>st</sup> Alco   | 2 <sup>nd</sup> Alco  |
| Signature  |  |
| (OVER)   |   |

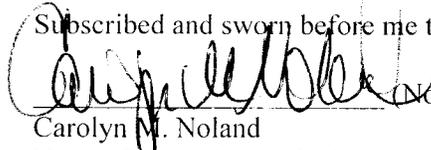
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 6<sup>th</sup> day of NOV., 2009.

  
Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130117

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130117

OCTOBER 13, 2009 ✓

OPERATOR'S NAME: *COB 10/13/09*  
VALERIO, KYLE D  
OPERATOR'S NUMBER: 2093  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
TEST

D.L. #: XXXXXX  
DEPT/AGENCY: KOD1  
CASE/REPORT: 2009000000  
TEST TYPE: V  
ALCO TARGET VALUE: .087 ✓  
ALCO S/N: X172933

--- BREATH ANALYSIS ---

|                                    |          |       |
|------------------------------------|----------|-------|
| .087 ADJUSTED FOR 29.86 in         |          |       |
| ALCO TARGET                        | .086     | 10:40 |
| BLANK TEST                         | .000     | 10:41 |
| INTERNAL STANDARD                  | VERIFIED | 10:41 |
| ALCO TV 29.86 in                   | .083     | 10:42 |
| BLANK TEST                         | .000 ✓   | 10:43 |
| SUBJECT SAMPLE <i>COB 10/13/09</i> | .080     | 10:43 |
| BLANK TEST                         | .000     | 10:44 |
| ALCO TV 29.86 in                   | .084 ✓   | 10:44 |
| BLANK TEST                         | .000     | 10:45 |

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130117

OCTOBER 13, 2009 ✓  
TIME 10:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/28/01  
HEATERS  
SAMPLE CHAMBER: 40c  
BREATH TUBE: 40c  
BAROMETER: 29.86 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#12 / \ \* + , - . : ; < > [ ] ^ \_ ` { | } ~ ? ! @ # \$ % & \* ( ) = > 70400DEF6  
ACXLR@PUBSCTUW 10/13/09 10:45:00  
report: 10/13/09 10:45