


MAR 29 2011

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130119</u> ✓
Name	<u>Robin P Brennan</u>	ID#	<u>4542</u> ✓
Date	<u>3-20-11</u> ✓		
A Agency	<u>Soldotna Police Dept</u>	Phone #	<u>262-4455</u>
Instrument Location	<u>Soldotna Police Dept</u>		
B Alco S/N	<u>X301536</u> ✓	Target Value	<u>.081</u> ✓
High Pressure	<u>600</u>		
Alco Test Values	<u>.083</u> ✓ 1st Alco	<u>.083</u> ✓ 2nd Alco	
Signature			


(OVER)

CRF
3/31/11


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

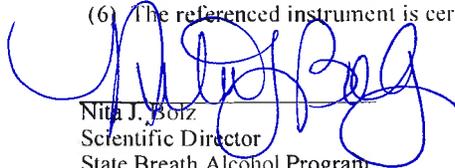
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 1st day of APRIL, 2010 DNW


 (Notary Seal Stamp)
 Daniel L. Nicholas
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130119

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130119

MARCH 20, 2011

CRF 3/31/11

OPERATOR'S NAME:

BRENNAN

OPERATOR'S NUMBER: 4542

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: UOC

DEPT/AGENCY: SLD1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .081

ALCO S/N: X301536

— BREATH ANALYSIS —

.081 ADJUSTED FOR 29.73 in

ALCO TARGET	.080	21:02
BLANK TEST	.000	21:03
INTERNAL STANDARD	VERIFIED	21:03
ALCO TU 29.73 in	.083	21:04
BLANK TEST	.000	21:05
SUBJECT SAMPLE	.000	21:05
BLANK TEST	.000	21:06
ALCO TU 29.73 in	.083	21:06
BLANK TEST	.000	21:07

CRF 3/31/11

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130119

MARCH 20, 2011

TIME 21:01

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 03/29/00

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 45c

BAROMETER: 29.73 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

F=PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z () ~ !