


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130119</u>
Name		<u>Tobin P Brennan</u>	ID# <u>4542</u> Date <u>10-28-08</u> ✓
A	Agency	<u>Soldotna Police Dept</u> ✓	Phone # <u>262-4435</u>
Instrument Location		<u>Soldotna PD</u>	<u>11-17-08 cmm</u>
Alco S/N		<u>X124650</u> ✓	Target Value <u>.074</u> ✓ High Pressure <u>1100</u> ✓
Alco Test Value Average		<u>.079</u> ✓	<u>.079</u> ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature		 ✓	
		CMB 11/18/08	

(OVER)

Under the Alaska Rules of Evidence, I certify that;



(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Tobin P Brennan, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

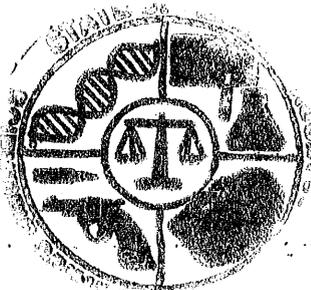

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

11/19/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130119 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

OCTOBER 28, 2008 *DOB 11/18/08*

OPERATOR'S NAME:

BRENNAN

OPERATOR'S NUMBER: 4542

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

UOC

O.L. #: UOC

DEPT/AGENCY: SLD1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .074 ✓

ALCO S/N: X124650

--- BREATH ANALYSIS ---

.074 ADJUSTED FOR 29.57 in  
ALCO TARGET .073 21:44  
BLANK TEST .000 21:45  
INTERNAL STANDARD VERIFIED 21:45  
ALCO TV 29.57 in .079 ✓ 21:46  
BLANK TEST .000 21:47  
SUBJECT SAMPLE *DOB 11/18/08* .000 21:47  
BLANK TEST .000 21:48  
ALCO TV 29.57 in .079 ✓ 21:48  
BLANK TEST .000 21:49

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

OCTOBER 28, 2008 ✓

TIME 21:42

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 03/29/00

HEATERS

SAMPLE CHAMBER: 40c

BREATH TUBE: 45c

BAROMETER: 29.57 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ■