

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130121

Supervisor/Operator Performing the Verification Procedure:

Name Matt McClurg ID# 6290 Date 2/4/08

A Agency Fairbanks Airport Police Phone # 474-2555

Instrument Location 6450 Airport Way, Ste 1, Fairbanks, AK 99709

B Alco S/N X301686 Target Value .082 High Pressure 800 psi

Alco Test Values .081 2/22/08
~~.080~~ 1st Alco .081 2nd Alco

Signature *Matt McClurg* COB
2/21/08

(OVER)

Under the Alaska Rules of Evidence, I certify that;


(Do Not write in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Matthew M McClurg, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

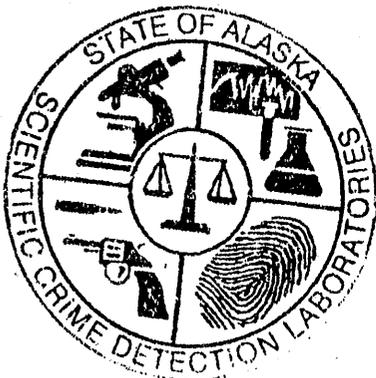

J Swartz 02/22/08
 Jeanne Swartz Date
 Scientific Director Designee
 State of Alaska
 State Breath Alcohol Testing Program

FEB 15 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130121

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

FEBRUARY 04, 2000

OPERATOR'S NAME:

MULLINS/MATT

OPERATOR'S NUMBER: 6253

SUBJECT'S LAST NAME:

UDC

SUBJECT'S FIRST NAME (I):

UDC

O.I.L. #: 1274567

DEPT/AGENCY: FBWS

DATE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .050

ALCO S/N: 2001655

--- BREATH ANALYSIS ---

.050 ADJUSTED FOR 29.67 in

ALCO TARGET	.051	22:14
BLANK TEST	.000	22:15
INTERNAL STANDARD	VERIFIED	22:15
ALCO TO 29.67 in	.051	22:15
BLANK TEST	.000	22:16
SUBJECT SAMPLE	.000	22:17
BLANK TEST	.000	22:18
ALCO TO 29.67 in	.050	22:18
BLANK TEST	.000	22:19

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

FEBRUARY 04, 2000
TIME 22:09

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 05/29/99

HEATERS

SAMPLE CHAMBER: 45c

BREATH TUBE: 45c

BAROMETER: 29.67 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

ALCO S/N: 2001655
ALCO S/N: 2001655
ALCO S/N: 2001655