

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130121</u>	
A	Name <u>Kyle Carrington</u>	ID# <u>5336</u> Date <u>10-5-08</u>	
	Agency <u>Fairbanks Airport Police & Fire</u>	Phone # <u>474-2555</u>	
	Instrument Location <u>5195 Brumbach Ave Fairbanks, AK 99709</u>		
B	Alco S/N <u>78895</u> ✓	Target Value <u>.081</u> ✓ High Pressure <u>900 PSI</u> ✓	
	Alco Test Values	<u>.079</u> ✓ 1 st Alco	<u>.080</u> ✓ 2 nd Alco
	Signature <u>[Handwritten Signature]</u> ✓		<u>CSB</u> <u>11/4/08</u>

(OVER)


Under the Alaska Rules of Evidence, I certify that (copy and paste in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kyle Carrington, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

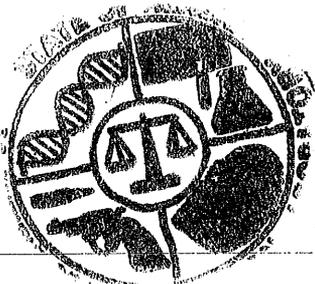

[Handwritten Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

11/5/08

Date

OCT 24 2008

BT9 06/03

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130121 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

OCTOBER 05, 2008 ✓ *11/1/08*

OPERATOR'S NAME:
CARRINGTON, KYLE
OPERATOR'S NUMBER: 5336
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/NI :

O.L. #: 0
DEPT/AGENCY: FBK6
CASE/REPORT: 0
TEST TYPE: U
ALCO TARGET VALUE: .001 ✓
ALCO S/N: 78895 ✓

— BREATH ANALYSIS —

.001 ADJUSTED FOR 29.12 in
ALCO TARGET .078 14:09
BLANK TEST .000 14:10
INTERNAL STANDARD VERIFIED 14:10
ALCO TU 29.12 in .079 14:10
BLANK TEST .000 14:11
SUBJECT SAMPLE .000 14:12
BLANK TEST .000 14:12
ALCO TU 29.12 in .000 ✓ 14:13
BLANK TEST .000 14:14

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

OCTOBER 05, 2008 ✓
TIME 14:06

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 03/29/00
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c
BAROMETER: 29.12 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxy{|}~■