

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 21 2010

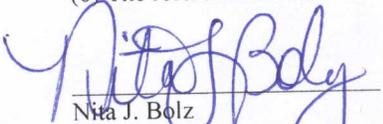
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130122
Name	Kirsten Hansen	ID#	KZH0
Date	05/19/2010		
A Agency	Alaska State Troopers / DJT0	Phone #	(907) 895-4800
Instrument Location	Delta Jct. Court House		
B Alco S/N	75602	Target Value	.081
High Pressure	950 psi		
Alco Test Values	0.079 .79	0.079 .79	
	1 st Alco 05/24/10	2 nd Alco 05/24/10	
Signature	Kirsten Hansen		003 5/24/10

(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 17th day of June, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130122

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130122 ✓

MAY 19, 2010 ✓

OPERATOR'S NAME: *CBS 5/24/10*
HANSEN/KIRSTEN/Z
OPERATOR'S NUMBER: 5440
SUBJECT'S LAST NAME: VERIF
SUBJECT'S FIRST NAME/MI :
OF CAL

O.L. #: 123456
DEPT.AGENCY: DJT0
CASE/REPORT: 09876
TEST TYPE: U
ALCO TARGET VALUE: .081 ✓
ALCO S/N: 75602 ✓

— BREATH ANALYSIS —

.081 ADJUSTED FOR 28.58 in ✓
ALCO TARGET .077 12:12
BLANK TEST .000 12:13
INTERNAL STANDARD VERIFIED 12:13
ALCO TV 28.58 in .079 12:13
BLANK TEST .000 12:14
SUBJECT SAMPLE *CBS 5/24/10* .000 12:15
BLANK TEST .000 12:15
ALCO TV 28.58 in .079 12:16
BLANK TEST .000 12:16

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130122 ✓

MAY 19, 2010 ✓
TIME 12:08

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 40c
BREATH TUBE: 40c
BAROMETER: 28.58 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNPOQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~