

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130122
Name	Kirsten Hansen	ID#	5440
		Date	11/11/2010
A Agency	Alaska State Troopers/DJT0	Phone #	(907) 895-4800
Instrument Location	Delta Jct. Court House		
B Alco S/N	75602	Target Value	.081
		High Pressure	915
Alco Test Values	0.078	0.078	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature	<i>Kirsten Hansen</i>		

(OVER)

*BMB  
12/16/10*

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>rd</sup> day of DEC, 2010.

*Daniel Nicholas* (Notary Seal Stamp)  
 Carolyn M. Notand  
 Notary Public, State of Alaska  
 Commission Expires with Office

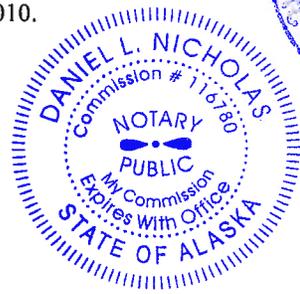

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130122

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130122

NOVEMBER 11, 2010

OPERATOR'S NAME:  
HANSEN/KIRSTEN/Z  
OPERATOR'S NUMBER: 5440  
SUBJECT'S LAST NAME:  
NOVEMBER  
SUBJECT'S FIRST NAME/MI :  
VOC/Z

O.L. #: 123456  
DEPT/AGENCY: DJT0  
CASE/REPORT: 10112010  
TEST TYPE: U  
ALCO TARGET VALUE: .061  
ALCO S/N: 75602

### — BREATH ANALYSIS —

.061 ADJUSTED FOR 28.42 in  
ALCO TARGET .076 21:04  
BLANK TEST .000 21:05  
INTERNAL STANDARD VERIFIED 21:05  
ALCO TV 28.42 in .078 21:06  
BLANK TEST .000 21:06  
SUBJECT SAMPLE .060 21:07  
BLANK TEST .000 21:08  
ALCO TV 28.42 in .078 21:08  
BLANK TEST .000 21:09

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130122

NOVEMBER 11, 2010  
TIME 21:10

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 28.40 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢