

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

NOV 28 2011

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

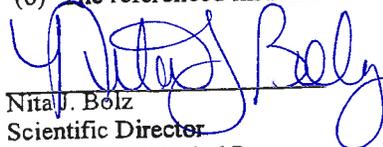
Supervisor/Operator Performing the Verification Procedure:	
Name	NICHOLAS YLTIEMET
ID#	3429
Date	11/18/11
Agency	METLAKATLA POLICE DEPT.
Phone	(907) 886-4011
Instrument Location	METLAKATLA POLICE DEPT.
DataMaster cdm S/N 130124	
Alco S/N	X172988
Target Value	.078
High Pressure	600psi
Alco Test Values	.078
1 st Alco	.078
2 nd Alco	
Signature	Nicholas Yltemet
	003 11/28/11

(OVER)


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of Feb, 2012.


Nikki Roth (Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130124

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130124

NOVEMBER 18, 2011 *COB 11/28/11*

OPERATOR'S NAME:
VLINIENT/NICHOLAS/L

OPERATOR'S NUMBER: 3429

SUBJECT'S LAST NAME:
UER

SUBJECT'S FIRST NAME/MI :
OF CAL

O.L. #: 0000

DEPT/AGENCY: MET1

CASE/REPORT: 0000

TEST TYPE: U

ALCO TARGET VALUE: .078

ALCO S/N: X172988

— BREATH ANALYSIS —

.078 ADJUSTED FOR 30.07 in		
ALCO TARGET	.078	10:13
BLANK TEST	.000	10:14
INTERNAL STANDARD	VERIFIED	10:14
ALCO TV 30.07 in	.078	10:14
BLANK TEST	.000	10:15
SUBJECT SAMPLE <i>COB</i>	.000	10:15
BLANK TEST <i>11/28/11</i>	.000	10:16
ALCO TV 30.07 in	.078	10:17
BLANK TEST	.000	10:17

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130124

NOVEMBER 18, 2011
TIME 10:10

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	42c
BAROMETER:	30.07 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ\]^_`abcde fghijklmno
pqrstuvwxyz{|}~||