

APR 01 2011

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130128

Name MALIK JONES ID# 5830 Date 3/25/11

A Agency AST Phone # 451-5100

Instrument Location CANTWELL

B Alco S/N 58442 Target Value .080 High Pressure 700 PST

Alco Test Values .074 .074
1st Alco 2nd Alco


Signature 

(OVER) AMB
4/1/11

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

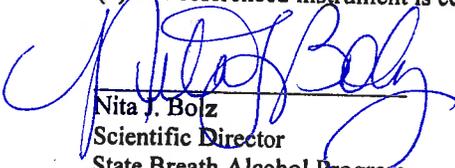
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 1st day of APRIL, 2011 DN

 (Notary Seal Stamp)
 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office

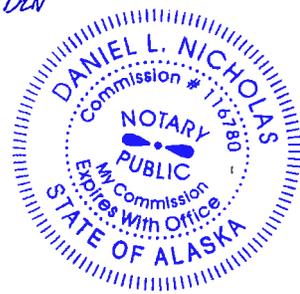

VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130128

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130128

MARCH 25, 2011

OPERATOR'S NAME: *BMB 4/11/11*
 JONES/HALIK/JAMAL
 OPERATOR'S NUMBER: 5830
 SUBJECT'S LAST NAME:
 VERIFICATION OF CAL
 SUBJECT'S FIRST NAME/NI :

U
 O.L. #: 1
 DEPT/AGENCY: CHT0
 CASE/REPORT:
 TEST TYPE: U
 ALCO TARGET VALUE: .000
 ALCO S/N: 58442

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 27.36 in		
ALCO TARGET	.073	22:00
BLANK TEST	.000	22:01
INTERNAL STANDARD	VERIFIED	22:01
ALCO TU 27.35 in	.074	22:02
BLANK TEST	.000	22:02
SUBJECT SAMPLE	.000	22:03
BLANK TEST	.000	22:04
ALCO TU 27.36 in	.074	22:04
BLANK TEST	.000	22:05

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130128

MARCH 25, 2011
 TIME 22:08

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	27.36 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; (=) ? @ A B C D E F G
 H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
 p q r s t u v w x y z { } ~ |