

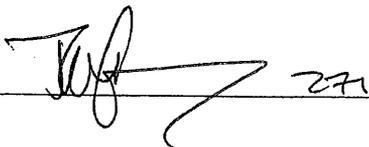
JAN 20 2009

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130130</u> ✓
Name		<u>JEREMY CONKLING</u>	ID# <u>6715</u> Date <u>01.24.09</u> ✓
A	Agency	<u>VALDEZ POLICE DEPARTMENT</u>	Phone # <u>835-4560</u>
Instrument Location		<u>VALDEZ JAIL</u>	✓
Alco S/N		<u>70108</u> ✓	Target Value <u>.083</u> ✓ High Pressure <u>980</u> ✓
Alco Test Value Average		<u>.081</u> ✓ 1 <sup>st</sup> Alco	<u>.081</u> ✓ 2 <sup>nd</sup> Alco
Signature			<u>CSB</u> <u>2/9/09</u>

(OVER)

Under the Alaska Rules of Evidence, I certify that;

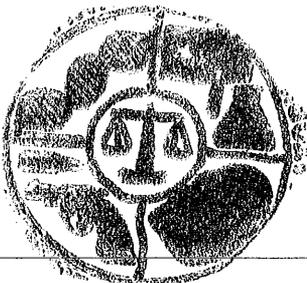
(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jeremy Conkling, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,



  
 \_\_\_\_\_  
 Jeanne Swartz  
 Scientific Director Designee  
 State of Alaska  
 State Breath Alcohol Testing Program

2/9/09  
Date

JAN 30 2009

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130130 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130130

JANUARY 24, 2009 ✓

OPERATOR'S NAME: *CAS 2/9/09*  
CONKLING  
OPERATOR'S NUMBER: 6715  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/NI :  
VOC

O.L. #: VOC  
DEPT/AGENCY: UPD1  
CASE/REPORT: VOC  
TEST TYPE: V  
ALCO TARGET VALUE: .083 ✓  
ALCO S/N: 76108

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.64 in		
ALCO TARGET	.085	17:06
BLANK TEST	.000	17:07
INTERNAL STANDARD	VERIFIED	17:07
ALCO TV 30.64 in	.081 ✓	17:07
BLANK TEST	.000	17:08
SUBJECT SAMPLE <i>CAS 2/9/09</i>	.000	17:09
BLANK TEST	.000	17:09
ALCO TV 30.64 in	.081 ✓	17:10
BLANK TEST	.000	17:11

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130130

JANUARY 24, 2009 ✓  
TIME 17:02

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	40c
BAROMETER:	30.64 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~#