

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 25 2009


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130130</u> ✓
Name	<u>Jeremy Conkling</u>	ID# <u>6715</u> Date <u>03.22.09</u> ✓
A Agency	<u>UPD</u>	Phone # <u>835 4560</u>
Instrument Location <u>UPD JAIL</u> ✓		
B Alco S/N <u>70108</u> ✓ Target Value <u>.083</u> ✓ High Pressure <u>720</u>		
Alco Test Value Average <u>.080</u> ✓ <u>.079</u> ✓		
1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco		
Signature <u>[Signature]</u> <u>271</u> ✓		<u>[Signature]</u> 4/14/09
(OVER)		

Under the Alaska Rules of Evidence, I certify that,

(Do Not write in the area below)

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jeremy Conkling, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

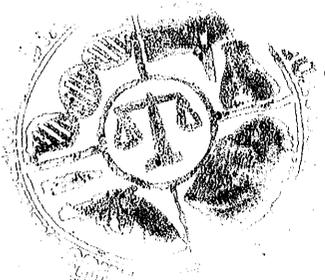

[Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

4/16/09

Date

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N 130130 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

### NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130130

MARCH 22, 2009

OPERATOR'S NAME: *CPB 4/14/09*  
 CONKLING  
 OPERATOR'S NUMBER: 6715  
 SUBJECT'S LAST NAME:

UOC  
 SUBJECT'S FIRST NAME/MI :  
 UOC

O.L. #: UOC  
 DEPT AGENCY: MPO1  
 CORE REPORT: UOC  
 TEST TYPE: U  
 ALCO TARGET VALUE: .083 ✓  
 ALCO S/N: 78187 ✓

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.04 in		
ALCO TARGET	.083	13:53
BLANK TEST	.000	13:54
INTERNAL STANDARD	0.000	13:54
ALCO TU 30.03 in	.083 ✓	13:55
BLANK TEST	.000	13:56
EXTERNAL SAMPLE	.083 ✓	13:56
BLANK TEST	.000	13:57
ALCO TU 30.04 in	.079 ✓	13:57
BLANK TEST	.000	13:58

### DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130130

MARCH 22, 2009 ✓  
 TIME 13:49

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
 PROGRAM: OKAY  
 SOFTWARE DATE: 02/20/01  
 HEATERS  
 SAMPLE CHAMBER: OK  
 BREATH TUBE: OK  
 BAROMETER: 30.03 in  
 FLOW DETECTOR: OKAY  
 PUMP  
 HIGH SPEED: OKAY  
 DETECTOR: OKAY  
 FILTERS: OKAY  
 QUARTZ STANDARD: OKAY  
 CALIBRATION: OKAY

PRINTER TEST

130130 130130 012345678910111213141516171819  
 ABCDEFGHIJKLMNOPQRSTUVWXYZ0123456789  
 abcdefghijklmnopqrstuvwxyz0123456789