

VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm Breath Test Instrument
 State of Alaska
 Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130131 ✓

Supervisor/Operator Performing the Verification Procedure:

Name Shayne Calt ID# 4559 Date 2-8-09 ✓

A Agency AST Phone # 733-2256

Instrument Location Talkeetna AST ✓

B Alco S/N X124665 ✓ Target Value .079 High Pressure 450

Alco Test Value Average .079 ✓ .078 ✓
 1st Alco 2nd Alco


Signature [Signature] CSB
3/24/09

Under the Alaska Rules of Evidence, I certify that: (OVER)

(a) I am ^(Do Not write in the area below) Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Shayne M Calt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

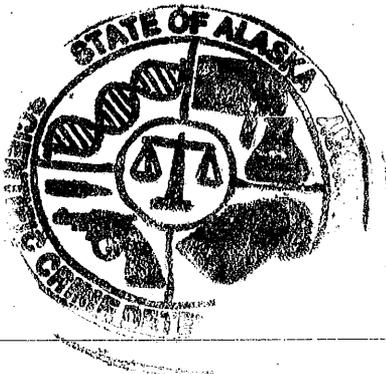

Signed and sealed,

[Signature] 3/24/09
 Jeanne Swartz Date
 Scientific Director Designee
 State of Alaska
 State Breath Alcohol Testing Program

FEB 24 2009

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130131 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130131

FEBRUARY 08, 2009 ✓

OPERATOR'S NAME:

CALT SHAYNE M

OPERATOR'S NUMBER: 4559

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI:

U

O.L. #: U

DEPT/AGENCY: TAL0

CASE/REPORT: U

TEST TYPE: U

ALCO TARGET VALUE: .079 ✓

ALCO S/N: X124665 ✓

BREATH ANALYSIS

.079 ADJUSTED FOR 29.46 in		
ALCO TARGET	.077	18:31
BLANK TEST	.000	18:32
INTERNAL STANDARD	VERIFIED	18:32
ALCO TV 29.46 in	.079 ✓	18:33
BLANK TEST	.000	18:34
SUBJECT SAMPLE	.000	18:34
BLANK TEST	.000	18:35
ALCO TV 29.46 in	.079 ✓	18:35

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130131

FEBRUARY 08, 2009 ✓
TIME 18:29

DIAGNOSTIC CHECK

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 41c
BAROMETER: 29.46 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! "# % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~