

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130131 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

[Empty box for taping]

Breath Test Record

Serial Number 130131 Model DataMaster
Location TALO AST/Talkeetna

Subject Information

Last Name Verificationofcal O.L. # V
First Name V

Operator Information

Operator Name Call Shayne M Case V
Operator # 4559 Department TALO

Test Results

Alco Target 0.079 Alco Serial X124665
Nominal 0.078 Barometer 29.83 Test Type V
Dry Gas 1 0.079 Time: 13:55:28 Test Date 05/20/2009
Subject Alcohol 0.000 Time: 13:57:06 Test Time 13:53:58
Dry Gas 2 0.079 Time: 13:58:22 Report Y

DIAGNOSTIC CHECK

[Empty box for taping]

Diagnostic Test Record

Serial Number 130131 Model DataMaster
Location TALO AST/Talkeetna

Diagnostic Test Results

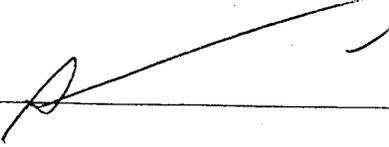
Test Date 05/20/2009 Computer Okay
Test Time 13:49:18 Program Okay
Software Date 02/20/2001
Sample Chamber (C) 49
Breath Tube (C) 42
Barometer (in) 29.85
Flow Detector Okay
High Speed Pump Okay
Detector Okay
Filter Okay
Quartz Okay
Calibration Okay

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

JUL 07 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130131</u> ✓
Name		<u>Shayne Calt</u>	ID# <u>4559</u> Date <u>5-20-09</u> ✓
A	Agency	<u>AST</u>	Phone # <u>733-2258</u>
Instrument Location		<u>Talkeetna AST</u>	✓
Alco S/N		<u>X124665</u> ✓	Target Value <u>.079</u> High Pressure <u>500</u>
B	Alco Test Value Average	<u>.079</u>	<u>.079</u>
		1 st Alco	2 nd Alco
Signature		 <u>7/15/09</u>	

(OVER)

BMB
7/14/09

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

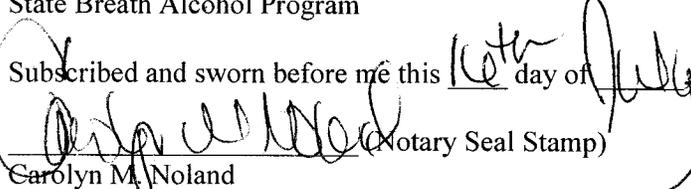
(Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.



Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 16th day of July 2009.


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

