

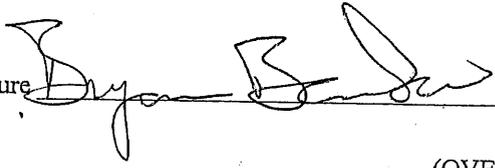
JUL 24 2007

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130133</u> ✓
Name	<u>BRYAN W. BARLOW</u>	ID#	<u>4548</u> ✓
		Date	<u>7/20/07</u> ✓
A	Agency	<u>Alaska State Troopers</u>	Phone # <u>907-783-0972</u>
	Instrument Location	<u>Girdwood AST</u>	
B	Alco S/N	<u>X173355</u> ✓	Target Value <u>.078</u> ✓
			High Pressure <u>1000</u>
	Alco Test Value Average	<u>.078</u> ✓	<u>.077</u> ✓
		1 st Alco	2 nd Alco
	Signature		<u>CBE</u>

(OVER)

Under the Alaska Rules of Evidence, I certify that: (Do Not Write in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Bryan W Barlow, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130133

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

JULY 20, 2007

OPERATOR'S NAME:
BARLOW BRYAN W
OPERATOR'S NUMBER: 4548
SUBJECT'S LAST NAME:
VERIFICATION
SUBJECT'S FIRST NAME/MI :
OF CALIBRATION
D.L. #: 123456
DEPT/AGENCY: GD40
CASE/REPORT: 07-12345
TEST TYPE: U
ALCO TARGET VALUE: .078
ALCO S/N: X173355

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 29.93 in		
ALCO TARGET	.083	18:42
BLANK TEST	.000	18:44
INTERNAL STANDARD	VERIFIED	18:44
ALCO TU 29.93 in	.078	18:44
BLANK TEST	.000	18:45
SUBJECT SAMPLE	.000	18:45
BLANK TEST	.000	18:46
ALCO TU 29.93 in	.077	18:46
BLANK TEST	.000	18:47

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

JULY 20, 2007
TIME 18:33

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	41c
BAROMETER:	29.93 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ #