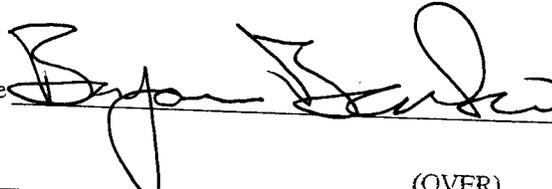


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

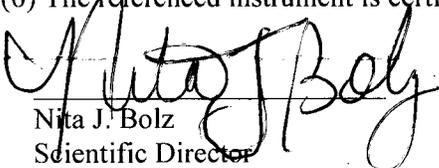
JAN 20 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program
JAN 12 2010

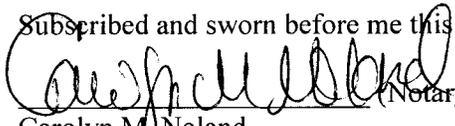
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130133
Name	BRYAN BARLOW	ID#	4548 Date 1/16/10
Agency	Alaska State Troopers	Phone #	907-783-0972
Instrument Location	Girdwood - AST		
Alco S/N		75260	Target Value .079 High Pressure 500
Alco Test Value Average		.076	.076
		1 st Alco	2 nd Alco
Signature			
(OVER)			

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory. (Do Not write in the area below)
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of January 2010.


(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N **130133**

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

JANUARY 16, 2010

OPERATOR'S NAME: *CBS*
BARLOW BRYAN W
OPERATOR'S NUMBER: 4540
SUBJECT'S LAST NAME:
OF CALIBRATION
SUBJECT'S FIRST NAME/MI :
VERIFICATION
O.L. #: 1234567
DEPT/AGENCY: 6040
CASE/REPORT: 10-12345
TEST TYPE: U
ALCO TARGET VALUE: .079
ALCO S/N: 73260

--- BREATH ANALYSIS ---

CBS
1/22/10

.079 ADJUSTED FOR 29.03 in		
ALCO TARGET	.076	19:29
BLANK TEST	.000	19:30
INTERNAL STANDARD	VERIFIED	19:30
ALCO TU 29.03 in	.076	19:31
BLANK TEST	.000	19:32
SUBJECT SAMPLE	.000	19:32
BLANK TEST	.000	19:33
ALCO TU 29.05 in	.076	19:33
BLANK TEST	.000	19:34

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

JANUARY 16, 2010
TIME 19:27

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c
BAROMETER: 29.03 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKL MNOPQRSTU VWXYZ[\]^_`'abcde fghijklmno
pqrstuvwxyz{|}~■