

SEP 14 2009

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N: 130134 ✓

Name CHRISTOPHER UMBS ID# 3669 Date 9/4/09 ✓

A Agency ALASKA STATE TROOPERS Phone # 465-4000

Instrument Location ANGCON PUBLIC SAFETY OFFICE ✓

---

B Alco S/N <sup>COB 9/24/09 70034</sup> ~~130300~~ ✓ Target Value .079 ✓ High Pressure 600 PSI

Alco Test Values .080 ✓ .080 ✓  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Handwritten Signature] ✓

COB  
9/25/09

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Handwritten Signature: Nita J. Bolz]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of Oct, 2009.

[Handwritten Signature: Carolyn M. Noland]  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

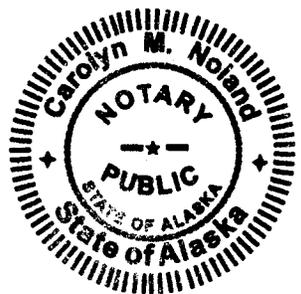

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130134

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130134

SEPTEMBER 04, 2009

OPERATOR'S NAME: *COS 9/26/09*  
UMBS/CHRISTOPHER/J  
OPERATOR'S NUMBER: 3669  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
L

O.L. #: L  
DEPT/AGENCY: AN60  
CASE/REPORT:  
TEST TYPE: T  
ALCO TARGET VALUE: .079 ✓  
ALCO S/N: ~~130300~~ *70034*  
*COS 9/24/09*

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.01 in ✓  
ALCO TARGET .079 12:15  
BLANK TEST .000 12:16  
INTERNAL STANDARD VERIFIED 12:16  
ALCO TU 30.01 in .000 ✓ 12:16  
BLANK TEST .000 12:17  
SUBJECT SAMPLE *COS 9/26/09* .000 12:18  
BLANK TEST .000 12:18  
ALCO TU 30.01 in .000 ✓ 12:19  
BLANK TEST .000 12:19

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130134

SEPTEMBER 04, 2009 ✓  
TIME 11:54

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.01 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@BCDEFG  
HIJKL MNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~