

1102 22 R4V

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130136</u>
Name <u>Daniel Gunderson</u>	ID# <u>6602</u>	Date <u>3-31-11</u>
A Agency <u>AST</u>	Phone # <u>543-2294</u>	
Instrument Location <u>BETHEL AST</u>		
Alco S/N <u>X124623</u>		Target Value <u>.081</u> High Pressure <u>9010</u>
Alco Test Values <u>.080</u>		<u>.079</u>
1 <sup>st</sup> Alco		2 <sup>nd</sup> Alco
Signature <u>[Handwritten Signature]</u>		

(OVER)

*[Handwritten initials]*  
4/25/11

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*[Handwritten Signature]*  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 27 day of MAY, 2011

*[Handwritten initials]*

*[Handwritten Signature]* (Notary Seal Stamp)  
 Carolyn M. Nolan KYLE KLOPPER  
 Notary Public, State of Alaska  
 Commission Expires with Office

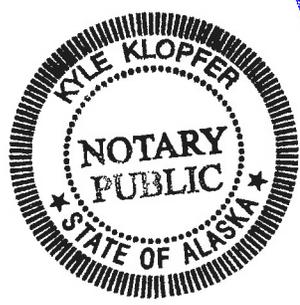

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130136

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130136

MARCH 31, 2011

OPERATOR'S NAME: GUNDERSON/DANIEL/G  
OPERATOR'S NUMBER: 6602  
SUBJECT'S LAST NAME: TEST  
SUBJECT'S FIRST NAME/MI: TEST  
O.L. #: 00  
DEPT/AGENCY: BETA  
CASE/REPORT: 00  
TEST TYPE: U  
ALCO TARGET VALUE: .001  
ALCO S/N: X124623

### --- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.96 in  
ALCO TARGET .001 11:22  
BLANK TEST .000 11:23  
INTERNAL STANDARD VERIFIED 11:24  
ALCO TU 29.96 in .000 11:24  
BLANK TEST .000 11:25  
SUBJECT SAMPLE .000 11:25  
BLANK TEST .000 11:26  
ALCO TU 29.96 in .079 11:26  
BLANK TEST .000 11:27

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130136

MARCH 31, 2011  
TIME 11:31

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.94 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKL/MNOPQRSTUWXYZ\]^\_`'abcdefghijklmnop  
qrstuvwxyz{|}~!@