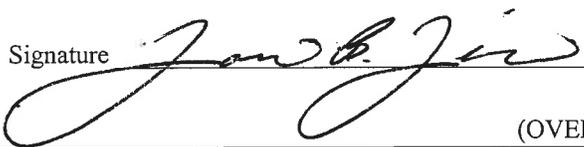


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

DEC 27 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N X 130141 CSB 12/30/10
Name: Lonnie Lewis	ID# 7130	Date 21 Dec 2010
A Agency 673 Security Forces Squadron	Phone # (907)-552-4661	
Instrument Location: Law Enforcement desk, Elmendorf AFB, AK		
B Alco S/N 27 ^{A090740} CSB 12/30/10	Target Value .083	High Pressure 1000 psi
Alco Test Values	0.082 1 st Alco	0.081 2 nd Alco
Signature 	CSB 12/30/10	

(Do not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10th day of MAR 2011

(Notary Seal Stamp)

Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130191

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130141

DECEMBER 21, 2010

OPERATOR'S NAME:
LEWIS/LONNIE/B

OPERATOR'S NUMBER: 7130

SUBJECT'S LAST NAME:

N/A

SUBJECT'S FIRST NAME/MI :

N/A

O.L. #: N/A

DEPT/AGENCY: EDF4

CASE/REPORT: 0000

TEST TYPE: U

ALCO TARGET VALUE: .003

ALCO S/N: A090740

— BREATH ANALYSIS —

.003 ADJUSTED FOR 29.73 in
ALCO TARGET .002 13:45
BLANK TEST .000 13:46
INTERNAL STANDARD VERIFIED 13:46
ALCO TV 29.73 in .002 13:46
BLANK TEST .000 13:47
SUBJECT SAMPLE .000 13:48
BLANK TEST .000 13:49
ALCO TV 29.73 in .001 13:49
BLANK TEST .000 13:50

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130141

DECEMBER 21, 2010

TIME 13:42

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 41c
BAROMETER: 29.75 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~■