

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

FEB 08 2008

Supervisor/Operator Performing the Verification Procedure: **DataMaster cdm S/N** 130142

Name John Martin ID# 6101 Date 1 February 08

**A** Agency Directorate of Emergency Services, FRN4 Phone # 384-3883

Instrument Location Bldg #656 A Street FT Richardson, AK 99505

**B** Alco S/N 78895 ✓ Target Value .075 ✓ High Pressure 500

Alco Test Values

<u>.076</u>	<u>.076</u>
1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco

Signature [Handwritten Signature] CSB  
2/21/08


(OVER)

Under the Alaska Rules of Evidence, I certify that (copy and paste in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Martin, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

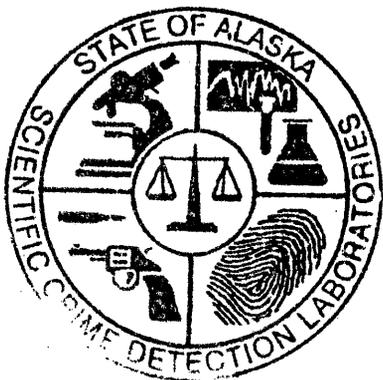

Signed and sealed

[Handwritten Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

02/22/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130142

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130142

FEBRUARY 01, 2008

OPERATOR'S NAME: *CAB 2/1/08*  
MARTIN/JOHN/B  
OPERATOR'S NUMBER: 6101  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :

NA  
O.L. #: NA  
DEPT/AGENCY: FRN4  
CASE/REPORT: NA  
TEST TYPE: U  
ALCO TARGET VALUE: .075  
ALCO S/N: 78895

--- BREATH ANALYSIS ---

*80/100*

.075 ADJUSTED FOR 29.62 in		
ALCO TARGET	.074	07:01
BLANK TEST	.000	07:02
INTERNAL STANDARD	VERIFIED	07:02
ALCO TV 29.62 in	.076	07:03
BLANK TEST	.000	07:04
SUBJECT SAMPLE	.000	07:04
BLANK TEST	.000	07:05
ALCO TV 29.62 in	.076	07:06
BLANK TEST	.000	07:06

*2/1/08*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130142

FEBRUARY 01, 2008  
TIME 07:07

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 03/29/00  
HEATERS  
SAMPLE CHAMBER: 43c  
BREATH TUBE: 43c  
BAROMETER: 29.62 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! "# \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~