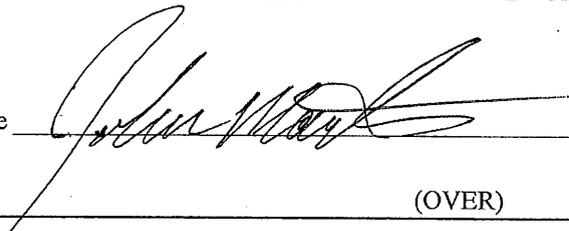


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130142 ✓			
Name	John Martin	ID#	6101	Date	15 April 08 ✓	
A Agency		Directorate of Emergency Services, FRN4 ✓	Phone #	384-3883		
Instrument Location						Bldg #656 A Street FT Richardson, AK 99505
B Alco S/N		78820 ✓	Target Value	.080 ✓	High Pressure	400
Alco Test Values		.079 ✓	.079 ✓			
		1 st Alco	2 nd Alco			
Signature					CSB 4/21/08	
(OVER)						


(Do Not write in the area below)
Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Martin, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

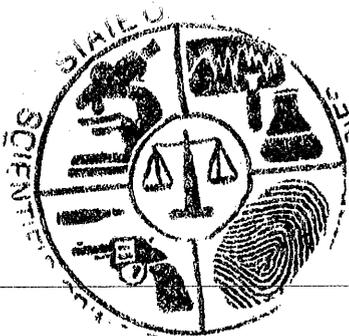



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

4/27/08

Date

BT9 APR 17 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130142

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

APRIL 15, 2008

OPERATOR'S NAME:
MARTIN/JOHN/B

OPERATOR'S NUMBER: 6101

SUBJECT'S LAST NAME:

VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
NA

O.L. #: NA

DEPT/AGENCY: FRM4

CASE/REPORT: NA

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: 78820

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.52 in
ALCO TARGET .078 06:25
BLANK TEST .000 06:26
INTERNAL STANDARD VERIFIED 06:26
ALCO TV 29.52 in .079 06:27
BLANK TEST .000 06:27
SUBJECT SAMPLE .000 06:28
BLANK TEST .000 06:29
ALCO TV 29.52 in .079 06:29
BLANK TEST .000 06:30

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

APRIL 15, 2008

TIME 06:30

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 03/29/00

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 44c

BAROMETER: 29.52 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~