

VERIFICATION OF CALIBRATION REPORT APR 30 2010
of DataMaster cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130142</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Scott E. Gardner</u>	ID# <u>6222</u> Date <u>4/24/10 BMB</u> <u>23 Apr 10 - 5/3/10</u> ✓
A Agency <u>Directorate of Emergency Services</u> Phone # <u>384-3888</u>	
Instrument Location <u>Bldg #656, A St, Ft Richardson, AK 99505</u> ✓	
B Alco S/N <u>555124</u> ✓ Target Value <u>.081</u> ✓ High Pressure <u>100 psi</u>	
Alco Test Values	<u>.083</u> ✓ 1 st Alco
	<u>.084</u> ✓ 2 nd Alco
Signature	
(OVER)	

BMB
5/3/10

(Do Not write in the area below)

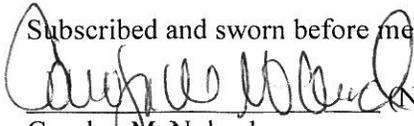
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program



Subscribed and sworn before me this 8th day of June, 2010.


 (Notary Seal Stamp)
 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130142 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142 ✓
APRIL 24, 2010 ✓
OPERATOR'S NAME: *BMB 5/3/10* BARNER/SCOTT E
OPERATOR'S NUMBER: 5222
SUBJECT'S LAST NAME: N/A
SUBJECT'S FIRST NAME/MI: N/A
CAL. #1 VERIFICATION OF CALIBRATION
DEPT/AGENCY: P/14
CASE REPORT#: N/A
TEST TYPE: U
ALCO TARGET VALUE: .081 ✓
ALCO S/N: 855124 ✓
--- BREATH ANALYSIS ---
ALCO ADJUSTED FOR 29.90 in ✓
ALCO TARGET .080 09111
BLANK TEST .000 09112
INTERNAL STANDARD VERIFIED 09112
ALCO TO 29.90 in .083 ✓ 09113
BLANK TEST .000 09113
SUBJECT SAMPLE *BMB 5/3/10* .081 ✓ 09114
BLANK TEST .000 09114
ALCO TO 29.90 in .084 ✓ 09115
BLANK TEST .000 09116

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142 ✓
APRIL 24, 2010 ✓
TIME 09:16 ✓
--- DIAGNOSTIC CHECK ---
COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 05/29/08
HEATERS
SAMPLE CHOUSER: 45c
BREATH TUBE: 45c
BAROMETER: 29.90 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY
PRINTER TEST
**#130142-1-0101055789114=090801076
HJKLWOPQRSTUWXYZ-101abodeight,9116
ScientificCrimeDetectionLab