

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

|  |  |
|--|--|
| DataMaster cdm S/N <u>130142</u> ✓   |  |
| Supervisor/Operator Performing the Verification Procedure:                       |  |
| Name <u>Ofc Lynne Gralewski-Baugus</u>   | ID# <u>6787</u> ✓ Date <u>8 Dec 2010</u> ✓                                       |
| A Agency <u>673 Security Forces Squadron</u> Phone # <u>552-3537</u>             |  |
| Instrument Location <u>Bldg 656 A Street, Joint Base Elmendorf-Richardson</u>    |  |
| B Alco S/N <u>X 172946</u> ✓ Target Value <u>.086</u> ✓ High Pressure <u>950</u> |  |
| Alco Test Values   | <u>.083</u> ✓<br>1st Alco  |
|  | <u>.082</u> ✓<br>2 <sup>nd</sup> Alco  |
| Signature  | <u>Lynne Gralewski-Baugus</u> <span style="float: right;">CB<br/>12/30/10</span> |
| (OVER)   |  |

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of JAN, 2011.

[Signature]  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

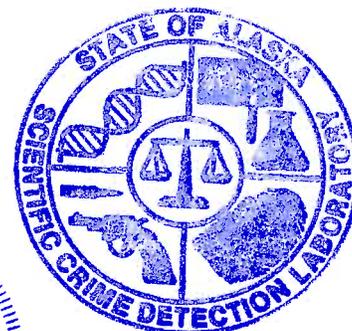

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130142

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130142

DECEMBER 08, 2010

OPERATOR'S NAME:  
GRALEWSKI-BAUGUS/LYNNE/M  
OPERATOR'S NUMBER: 6282

SUBJECT'S LAST NAME:  
VERIFICATION OF CALIBRATION  
SUBJECT'S FIRST NAME/MI :  
UOC

D.L. #: NONE  
DEPT/AGENCY: ED-F4  
CASE/REPORT: NONE  
TEST TYPE: U  
ALCO TARGET VALUE: 0.086  
ALCO S/N: X172946

--- BREATH ANALYSIS ---

.086 ADJUSTED FOR 29.41 in  
ALCO TAPSET .084 10:46  
BLANK TEST .000 10:47  
INTERNAL STANDARD VERIFIED 10:47  
ALCO TV 29.41 in .083 10:47  
BLANK TEST .000 10:48  
SUBJECT SAMPLE .000 10:49  
BLANK TEST .000 10:50  
ALCO TV 29.41 in .082 10:51  
BLANK TEST .000 10:51

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130142

DECEMBER 08, 2010  
TIME 10:42

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 03/29/00  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 44c  
BAROMETER: 29.41 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEFB  
HIJKLNPQRSTUWVXYZ[-]\_`'abcdefghijklmnop  
pqrstuvwxyz{|}~■