

OCT 06 2009

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska  
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130143 ✓

Name WADE TOLLIVER ID# 3805 DWC Date 22 Sept 09

A Agency FTWAIN WRIGHT POLICE Phone # 907 353-7553

Instrument Location BIDG 3028 ✓

---

B Alco S/N X 301755 Target Value .082 High Pressure 200 psi

Alco Test Values .088 ✓ .087 ✓

1<sup>st</sup> Alco                      2<sup>nd</sup> Alco

Signature [Signature]

(OVER)

*[Handwritten initials]*  
10/13/09

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22<sup>nd</sup> day of Oct, 2009.

[Signature] (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

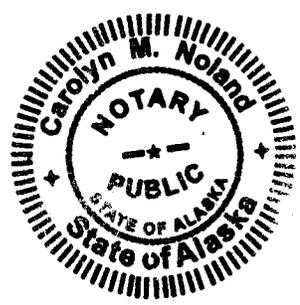

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130143 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130143

SEPTEMBER 21, 2009

OPERATOR'S NAME:  
TOLLIVER, WADE L  
OPERATOR'S NUMBER: 3805  
SUBJECT'S LAST NAME:  
DOE  
SUBJECT'S FIRST NAME/MI :  
JOHN N  
O.L. #: 000000000  
DEPT/AGENCY: FA14  
CASE/REPORT:  
TEST TYPE: T  
ALCO TARGET VALUE: .002 ✓  
ALCO S/N: K301755 ✓

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.23 in  
ALCO TARGET .000 13:11  
BLANK TEST .000 13:13  
INTERNAL STANDARD (VERIFIED) 13:13  
ALCO TU 29.23 in .000 13:13  
BLANK TEST .000 13:14  
SUBJECT SAMPLE .000 13:14  
BLANK TEST .000 13:15  
ALCO TU 29.23 in .007 13:15  
BLANK TEST .000 13:16

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130143

SEPTEMBER 21, 2009 ✓  
TIME 13:18

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.23 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢