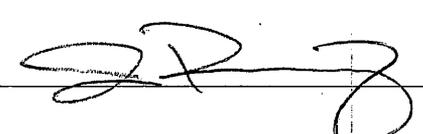


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N 130144 ✓
Name: Jose Ramirez	ID# 6532	Date: December 05, 2008 ✓
A Agency: 3 <sup>rd</sup> Security Forces Squadron	Phone # 552-6570	
Instrument Location: Bldg 8517, Law Enforcement Desk, Elmendorf AFB, AK ✓		
B Alco S/N 57345 ✓	Target Value .086 ✓	High Pressure 1200psi
Alco Test Values	.080 ✓ 1 <sup>st</sup> Alco	.079 ✓ 2 <sup>nd</sup> Alco
Signature		COS 12/23/08
(OVER)		


Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jose A Ramirez, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

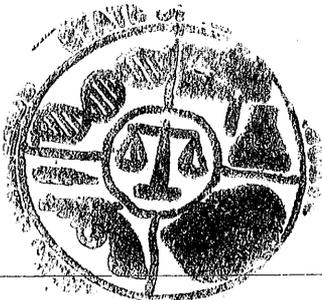

  
\_\_\_\_\_  
Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

12/23/08  
\_\_\_\_\_  
Date

BT9 03/00

DEC 12 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130144 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144

DECEMBER 05, 2008 ✓

OPERATOR'S NAME: *CAB 12/3/08*  
RAMIREZ/JOSE/A  
OPERATOR'S NUMBER: 6532  
SUBJECT'S LAST NAME:  
VOC  
SUBJECT'S FIRST NAME/MI :  
VOC  
O.L. #: 1234567890  
DEPT/AGENCY: EDF4  
CASE/REPORT: 20081205  
TEST TYPE: U  
ALCO TARGET VALUE: .006 ✓  
ALCO S/N: 57345

### --- BREATH ANALYSIS ---

.006 ADJUSTED FOR 29.68 in		
ALCO TARGET	.005	14:36
BLANK TEST	.000	14:37
INTERNAL STANDARD	VERIFIED	14:37
ALCO TV 29.68 in	.000 ✓	14:37
BLANK TEST	.000	14:38
SUBJECT SAMPLE <i>CAB 12/3/08</i>	.000	14:38
BLANK TEST	.000	14:39
ALCO TV 29.68 in	.079 ✓	14:39
BLANK TEST	.000	14:40

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144

DECEMBER 05, 2008 ✓  
TIME 14:33

### --- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	42c
BAROMETER:	29.70 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrs tuvwxyz{|}~#