

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <del>X</del> 130144 <i>DMW</i> <i>12/16/10</i>
A	Name: Lonnie Lewis ID# 7130	Date 15 Dec 2010
	Agency 673 Security Forces Squadron	Phone # (907)-552-4661
	Instrument Location: Law Enforcement desk, Elmendorf AFB, AK	
B	Alco S/N 2T	Target Value .080 ✓ High Pressure
	Alco Test Values	0.079 ✓ 1 <sup>st</sup> Alco
		0.078 ✓ 2 <sup>nd</sup> Alco
	Signature <i>[Handwritten Signature]</i>	
	(OVER)	<i>BMB</i> <i>12/23/10</i>


I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*[Handwritten Signature]*  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of JAN, 2011 *DMW*

*[Handwritten Signature]*  
 (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

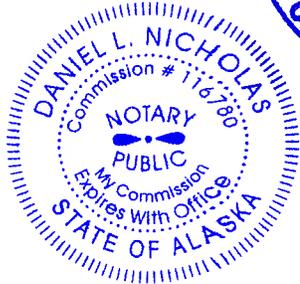

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N ~~X~~130144

*12/16/10*

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144

DECEMBER 15, 2010

OPERATOR'S NAME:

LEWIS

OPERATOR'S NUMBER: 7130

SUBJECT'S LAST NAME:

LEWIS

SUBJECT'S FIRST NAME/MI :

LANNIE

D.L. #: NA

DEPT/AGENCY: EDF4

CASE/REPORT: NA

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: 2T

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.72 in  
ALCO TARGET .079 09:40  
BLANK TEST .000 09:42  
INTERNAL STANDARD VERIFIED 09:42  
ALCO TV 29.72 in .079 09:42  
BLANK TEST .000 09:43  
SUBJECT SAMPLE .000 09:43  
BLANK TEST .000 09:44  
ALCO TV 29.72 in .078 09:44  
BLANK TEST .000 09:45

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144

DECEMBER 15, 2010

TIME 09:53

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS:  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.73 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#\$%^&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKL MNOPQRSTUVWXYZ\|\_`'abcde fghijklano  
pqrstuvwxyz{|}~