


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DEC 21 2009

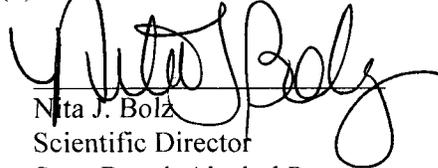
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>180171</u> ✓
Name	<u>Gregory Vermore</u>	ID# <u>6691</u> Date <u>4/10/2007</u> ✓
A Agency	<u>E14</u>	Phone # <u>2937</u>
Instrument Location	<u>Rm 143</u>	
B Alco S/N	<u>58428</u>	Target Value <u>.080</u> High Pressure <u>29.02</u>
Alco Test Values	<u>.082</u> 1 <sup>st</sup> Alco	<u>.083</u> 2 <sup>nd</sup> Alco
Signature		
(OVER)		

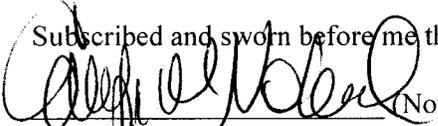
8MB  
1/5/10

(Do Not write in the area below)

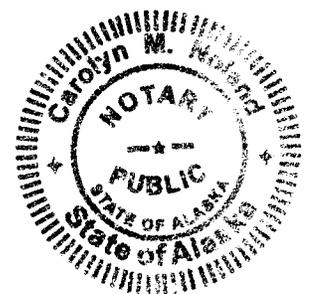
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 7<sup>th</sup> day of May 2010  
 (Notary Seal Stamp)

Carolyn M. Nofand  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130171 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

<b>Breath Test Record</b>	
Serial Number	130171
Model	DataMaster
Location	EIL4
	Eielson AFB/354 SFS
<b>Subject Information</b>	
Last Name	Voc
O.L. #	N/A
First Name	Voc
<b>Operator Information</b>	
Operator Name	Lormore/Gregory
Case	VOC
Operator #	6691
Department	EIL4
<b>Test Results</b>	
Alco Target	.080 ✓
Alco Serial	58428
Nominal	0.077
Barometer	29.02
Test Type	V ✓
Dry Gas 1	0.082 ✓
Time:	13:56:14
Test Date	04/10/2009
Subject Alcohol	0.000 ✓
Time:	13:57:31
Test Time	13:53:49
Dry Gas 2	0.083 ✓
Time:	13:58:53
Report	Y

## DIAGNOSTIC CHECK

<b>Diagnostic Test Record</b>	
Serial Number	130171
Model	DataMaster
Location	EIL4
	Eielson AFB/354 SFS
<b>Diagnostic Test Results</b>	
Test Date	04/10/2009 ✓
Computer	Okay
Test Time	13:51:21
Program	Okay
Software Date	02/20/2001
Sample Chamber (C)	49
Breath Tube (C)	41
Barometer (in)	29.02
Flow Detector	Okay
High Speed Pump	Okay
Detector	Okay
Filter	Okay
Quartz	Okay
Calibration	Okay

BMB  
1/5/10