

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
 State of Alaska  
 Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: <span style="float: right;">DataMaster cdm S/N <u>13017T</u> ✓</span>	
Name <u>CHRISTOPHER CHAPMAN</u>	ID# <u>6390</u> Date <u>22 Jul 08</u> ✓
A Agency <u>E164</u> Phone # <u>907-377-1408</u>	
Instrument Location <u>354 SFS 1451 DIVISION ST. EIELSON AFB, AK</u> <span style="float: right;"><u>99702</u></span>	
B Alco S/N <u>X301542</u> ✓ Target Value <u>.075</u> ✓ High Pressure <u>800</u>	
Alco Test Values <u>.079</u> ✓ 1 <sup>st</sup> Alco	<u>.080</u> ✓ 2 <sup>nd</sup> Alco
Signature 	<u>CSB</u> <u>7/25/08</u>

(OVER)


Under the Alaska Rules of Evidence, I certify that;

(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Christopher M Chapman, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

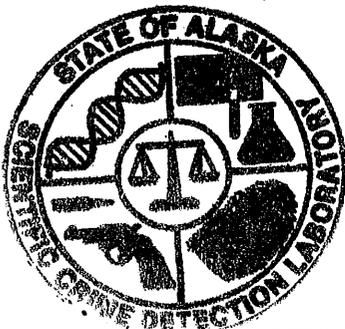

Signed and sealed,



Jeanne Swartz  
 Scientific Director Designee  
 State of Alaska  
 State Breath Alcohol Testing Program

7/28/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130171 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130171

JULY 22, 2008 ✓  
7/25/08

OPERATOR'S NAME:  
CHARMAN CHRISTOPHER M  
OPERATOR'S NUMBER: 6390  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/NI :  
VOC

O.L. #: 1  
DEPT/AGENCY: ETL4  
CASE/REPORT:  
TEST TYPE: U  
ALCO TARGET VALUE: .075 ✓  
ALCO S/N: X301542 ✓

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 29.54 in  
ALCO TARGET .074 13:34  
BLANK TEST .000 13:35  
INTERNAL STANDARD VERIFIED 13:35  
ALCO TV 29.54 in .079 ✓ 13:36  
BLANK TEST .000 ✓ 13:36  
SUBJECT SAMPLE .000 ✓ 13:37  
BLANK TEST .000 13:38  
ALCO TV 29.54 in .080 ✓ 13:38  
BLANK TEST .000 13:39

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130171

JULY 22, 2008 ✓  
TIME 13:40

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 43c  
BAROMETER: 29.54 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~#