

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DEC 21 2009

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130171

A Name Gregory S. Verma C ID# 66691 Date 7/28/09  
Agency E:14 Phone # 122291 2833  
Instrument Location ASR-143

B Alco S/N 58428 Target Value 0.080 High Pressure 27.88

Alco Test Values 0.082 ✓ 0.082 ✓  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature]


(OVER) [Signature] 1/5/10

(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 7th day of January 2010  
[Signature] (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

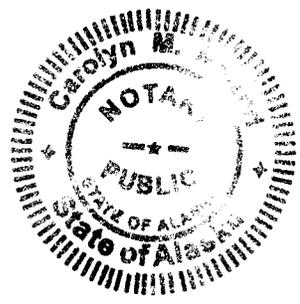

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130171 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

### Breath Test Record

Serial Number 130171 Model DataMaster  
Location EIL4 Eielson AFB/354 SFS

### Subject Information

Last Name Voc O.L. # VOC  
First Name V

### Operator Information

Operator Name Lormore/Gregory Case VOC  
Operator # 6691 Department EIL4

### Test Results

Alco Target .080 Alco Serial 58428  
Nominal 0.079 Barometer 29.88 Test Type V  
Dry Gas 1 0.082 Time: 09:53:47 Test Date 07/28/2009 ✓  
Subject Alcohol 0.000 Time: 09:55:06 Test Time 09:52:02  
Dry Gas 2 0.082 Time: 09:56:47 Report Y

## DIAGNOSTIC CHECK

### Diagnostic Test Record

Serial Number 130171 Model DataMaster  
Location EIL4 Eielson AFB/354 SFS

### Diagnostic Test Results

Test Date 07/28/2009 ✓  
Test Time 09:45:13  
*AMB 115110*  
Computer Okay  
Program Okay  
Software Date 02/20/2001  
Sample Chamber (C) 49  
Breath Tube (C) 41  
Barometer (in) 29.88  
Flow Detector Okay  
High Speed Pump Okay  
Detector Okay  
Filter Okay  
Quartz Okay  
Calibration Okay