

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130172

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

<b>Breath Test Record</b>	
Serial Number	130172
Model	DataMaster
Location	TOKO
	AST/Tok

*COB 12/17/09*

<b>Diagnostic Test Record</b>	
Serial Number	130172
Model	DataMaster
Location	TOKO
	AST/Tok

<b>Subject Information</b>	
Last Name	Verif
O.L. #	000000
First Name	Of Cal

<b>Diagnostic Test Results</b>	
Test Date	05/21/2009
Test Time	12:19:23
Computer	Okay
Program	Okay
Software Date	02/20/2001
Sample Chamber (C)	48
Breath Tube (C)	43
Barometer (in)	29.65
Flow Detector	Okay
High Speed Pump	Okay
Detector	Okay
Filter	Okay
Quartz	Okay
Calibration	Okay

<b>Operator Information</b>	
Operator Name	Johnson Brent W
Case	00-000
Operator #	4980
Department	TOKO

<b>Test Results</b>	
Alco Target	.083
Alco Serial	X173017
Nominal	0.082
Barometer	29.65
Test Type	V
Dry Gas 1	0.083
Time	12:23:14
Test Date	05/21/2009
Subject Alcohol	0.000
Time	12:24:40
Test Time	12:21:54
Dry Gas 2	0.084
Time	12:25:45
Report	Y

*COB 12/17/09*

# VERIFICATION OF CALIBRATION REPORT

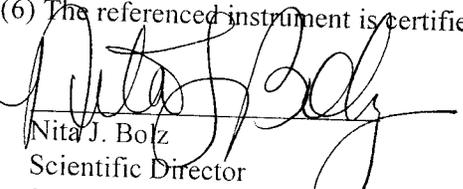
of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130172
Name	Brent Johnson	ID#	4980
		Date	5/21/09
A	Agency	AST	Phone #
	Instrument Location	AST - Tok	
Alco S/N		Target Value	High Pressure
X173017		0.083	900
B	Alco Test Values	0.083	0.084
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			
(OVER)			

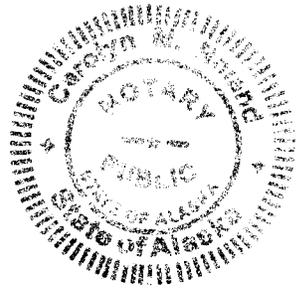
(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of Dec, 2009.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



12/12/2009 10:41 8088790676 MAJISUNSET