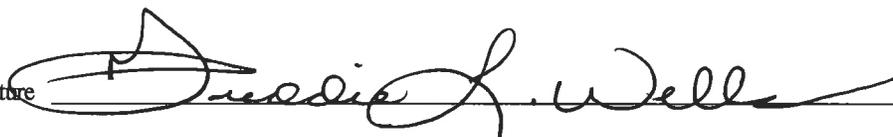


# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


DataMaster cdm S/N <u>130172</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Sgt. Freddie Wells</u>	ID# <u>4246</u> Date <u>9-10-200</u> ✓
A Agency <u>Alaska State Troopers</u> Phone # <u>(907) 883-5454</u>	
Instrument Location <u>Tok, Alaska</u>	
B Alco S/N <u>X173017</u> ✓ Target Value <u>.083</u> ✓ High Pressure <u>650 PSI</u>	
Alco Test Values	<u>.083</u> ✓ 1 <sup>st</sup> Alco
	<u>.082</u> ✓ 2 <sup>nd</sup> Alco
Signature	
	(OVER)

*BMB  
9/23/10*

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

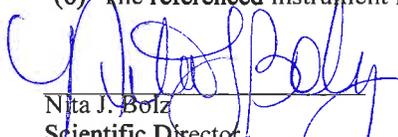  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 9<sup>th</sup> day of Nov, 2010.

 (Notary Seal Stamp)

Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130172

BMB  
9/23/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130172

SEPTEMBER 10, 2010

OPERATOR'S NAME:  
WELLS/FREDDIE/L  
OPERATOR'S NUMBER: 4246  
SUBJECT'S LAST NAME:  
VOC  
SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: 00000000  
DEPT/AGENCY: TOKO  
CASE/REPORT: VOC  
TEST TYPE: V  
ALCO TARGET VALUE: .083  
ALCO S/N: X173017

### — BREATH ANALYSIS —

.083 ADJUSTED FOR 28.52 in  
ALCO TARGET .079 16:20  
BLANK TEST .000 16:21  
INTERNAL STANDARD VERIFIED 16:21  
ALCO TV 28.52 in .083 16:21  
BLANK TEST .000 16:22  
SUBJECT SAMPLE .000 16:22  
BLANK TEST .000 16:23  
ALCO TV 28.52 in .082 16:23  
BLANK TEST .000 16:24

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130172

SEPTEMBER 10, 2010  
TIME 16:38

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 28.52 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMN0PQRSTUWXYZ[\]^\_`abcdefgijklmno  
pqrs tuvwxyz{|}~■