

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130173

Supervisor/Operator Performing the Verification Procedure:
 Name Peter Steen ID# 4572 Date 04/09/2011
12/31/12

A Agency AST 1 BHP PRO Phone # 352-5401
 Instrument Location Glenallen

B Alco S/N 78820 Target Value .083 High Pressure 600

Alco Test Values .079 1.079
 1st Alco 2nd Alco

Signature [Signature]

(OVER)

BMB
6/13/11

BMB
6/13/11

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 16 day of JUNE, 2010. NJB

[Signature] (Notary Seal Stamp)
 Daniel L. Nicholas KYLE KLOPPER
 Notary Public, State of Alaska
 Commission Expires with Office

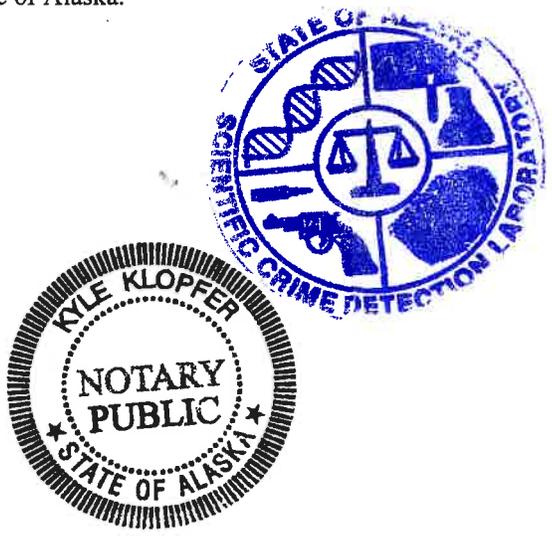

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130173

Bmb
6/13/11

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130173
APRIL 09, 2011
OPERATOR'S NAME: STEEN, PETER C
OPERATOR'S NUMBER: 4572
SUBJECT'S LAST NAME: VOC
SUBJECT'S FIRST NAME/MI: VOC
O.L. #: VOC
DEPT/AGENCY: PALT
CASE/REPORT: U
TEST TYPE: U
ALCO TARGET VALUE: .083
ALCO S/N: 78828

— BREATH ANALYSIS —

.083 ADJUSTED FOR 27.87 in		
ALCO TARGET	.077	16:30
BLANK TEST	.000	16:31
INTERNAL STANDARD	VERIFIED	16:31
ALCO TV 27.87 in	.079	16:32
BLANK TEST	.000	16:33
SUBJECT SAMPLE	.000	16:33
BLANK TEST	.000	16:34
ALCO TV 27.87 in	.079	16:34
BLANK TEST	.000	16:35

Bmb
6/13/11

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130173
APRIL 09, 2011
TIME 16:27

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 27.87 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJ.KLMNOPQRSTUVWXYZ\]^_`abcdefgijklmnop
qrs'tuvwxyz{|}~■

Bmb
6/13/11