

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130173</u> ✓
Name		<u>J Heinbaugh</u>	ID# <u>5828</u> Date <u>9-1-08</u> ✓
A	Agency	<u>AST</u>	Phone # <u>822-3263</u>
Instrument Location <u>Glennallen</u>			
Alco S/N		<u>77198</u> ✓ <del>130173</del> <u>9/1/08</u> ✓	Target Value <u>0.083</u> ✓ High Pressure <u>100</u>
Alco Test Values		<u>0.078</u> ✓ 1 <sup>st</sup> Alco	<u>0.079</u> ✓ 2 <sup>nd</sup> Alco
Signature		<u>[Signature]</u>	<u>CSB</u> <u>9/12/08</u>

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Josh Heinbaugh, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

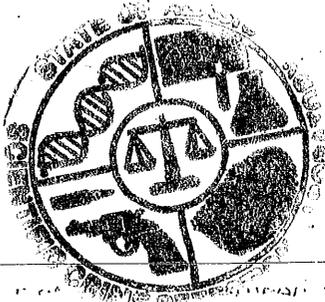

[Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

9/15/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130173 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130173

SEPTEMBER 01, 2008 *CS 9/12/08*

OPERATOR'S NAME:  
HEINBAUGH  
OPERATOR'S NUMBER: 5828  
SUBJECT'S LAST NAME:  
UC  
SUBJECT'S FIRST NAME/MI :  
UC

D.L. #: UOC  
DEPT/AGENCY: GAKB  
CASE/REPORT: UOC  
TEST TYPE: U  
ALCO TARGET VALUE: 0.083 ✓  
ALCO S/N: 77198 ✓

### — BREATH ANALYSIS —

.083 ADJUSTED FOR 28.30 in		
ALCO TARGET	.078	16:39
BLANK TEST	.000	16:40
INTERNAL STANDARD	VERIFIED	16:40
ALCO TV 28.30 in	.078 ✓	16:40
BLANK TEST	.000	16:41
SUBJECT SAMPLE	.000 <i>CS 9/12/08</i>	16:42
BLANK TEST	.000	16:43
ALCO TV 28.30 in	.079 ✓	16:43
BLANK TEST	.000	16:44

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130173

SEPTEMBER 01, 2008 ✓  
TIME 17:20

### — DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	28.29 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKL MNOPQRSTUVWXYZ\]^\_`'abcde fghijklmnp  
q rstuvwxyz{|}~