

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130173</u> ✓
Name	<u>Josh Heimbaugh</u>	ID# <u>5823</u> ✓ Date <u>12-8-10</u> ✓
A Agency	<u>AST</u>	Phone # <u>822-3263</u>
Instrument Location <u>Glennallen</u>		
Alco S/N <u>X124669</u> ✓		Target Value <u>0.083</u> ✓ High Pressure <u>200</u>
Alco Test Values		
	<u>0.081</u> ✓ 1st Alco	<u>0.082</u> ✓ 2nd Alco
Signature <u>[Signature]</u>		

(OVER)

BMB
12/16/10

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of JAN, 2011

[Signature] (Notary Seal Stamp)

Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

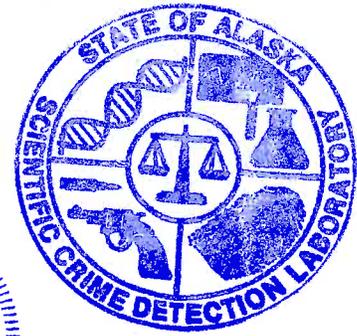

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130173

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130173

DECEMBER 08, 2010

OPERATOR'S NAME:
HEINDALGH

OPERATOR'S NUMBER: 5828

SUBJECT'S LAST NAME:
UOC

SUBJECT'S FIRST NAME/MI :
UOC

O.L. #: UOC

DEPT/AGENCY: ANK0

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: 0.083

ALCO S/N: X124669

— BREATH ANALYSIS —

.083 ADJUSTED FOR 28.19 in
ALCO TARGET .078 11:31
BLANK TEST .000 11:32
INTERNAL STANDARD VERIFIED 11:32
ALCO TV 28.19 in .081 11:33
BLANK TEST .000 11:33
SUBJECT SAMPLE .000 11:34
BLANK TEST .000 11:35
ALCO TV 28.19 in .082 11:35
BLANK TEST .000 11:36

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130173

DECEMBER 08, 2010
TIME 11:37

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 28.19 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghi jklmno
pqrstuvwxyz{|}~•