

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N <u>130174</u> ✓	
Name <u>Steve Christensen</u>	ID# <u>1315</u> Date <u>4/3/06</u> ✓
Agency <u>Juneau Police Dept</u>	Phone # <u>907-586-0600</u>
Instrument Location <u>Juneau Police Dept</u>	
Alco S/N <u>78964</u> ✓ Target Value <u>.083</u> ✓ High Pressure <u>500</u>	
Alco Test Value Average <u>.081</u> ✓ 1 <sup>st</sup> Alco	<u>.082</u> ✓ 2 <sup>nd</sup> Alco
Signature <u>[Handwritten Signature]</u>	C.O.B. 4/12/06 CBE


(OVER)

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

- (a) I am Chris W. Beheim, Director, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve Christensen, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

Chris W. Beheim ✓ 4-12-06  
Chris W. Beheim Date  
Scientific Director  
State of Alaska  
State Breath Alcohol Testing Program

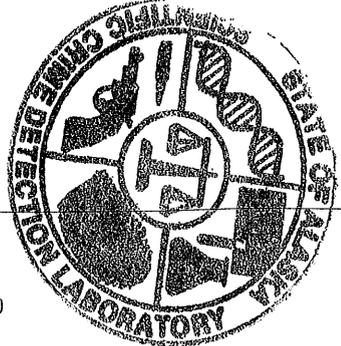

APR 10 2006

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130174

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130174

APRIL 03, 2006 *C.O.B. 4/12/06*

OPERATOR'S NAME: CHRISTENSEN, S,E  
OPERATOR'S NUMBER: 1315  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI : VOC

O.L. #: 040306  
DEPT/AGENCY: JNU1  
CASE/REPORT: 040306  
TEST TYPE: V  
ALCO TARGET VALUE: .083  
ALCO S/N: 78966

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.40 in		
ALCO TARGET	.084	04:17
BLANK TEST	.000	04:19
INTERNAL STANDARD	VERIFIED	04:19
ALCO TV 30.40 in	.081	04:19
BLANK TEST	.000	04:20
SUBJECT SAMPLE	.000 <i>C.O.B. 4/12/06</i>	04:21
BLANK TEST	.000	04:21
ALCO TV 30.40 in	.082	04:22
BLANK TEST	.000	04:23

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130174

APRIL 03, 2006  
TIME 04:23

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	40c
BAROMETER:	30.42 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstu  
vwxyz{|}~\*~